

## Fixed Length Medical Ceiling Column


### SPECIFICATION

#### Fixed Length Medical Ceiling Column

##### Model Number CCF2-XX-YY

The column shall be 11.5" square and fabricated from steel, with all edges and surfaces having a powder coat finish. Two (2) 17.3" cornices shall be provided to trim the upper column shroud to the finished ceiling. The cornices shall have 1/2" adjustment to compensate for variations in the finished ceiling thickness. The shrouds shall be removable for inspection of piping and internal wiring. The entire column shall be supported from a seven gauge steel mounting plate. The mounting plate shall have four (4) 3/4" diameter holes, one in each corner for attachment to structural ceiling support provided by others. Structural supports for the column shall be securely attached to structural members and be capable of supporting a minimum 400 lb load. Gas outlets shall be supplied with 1/2" OD (3/8" nominal) type K copper extension tubes to allow for silver solder connection to the piping system. Copper tubing shall extend a minimum of 7" from the lower face of the column.


BeaconMedaes ceiling columns will accommodate Series B Diameter Index Safety System (DISS), Geometric, Pin Index or Latch type, quick connect medical outlets. Electrical outlets can be hospital grade duplex or Hubbellock® receptacles. Bottom and side mounted services shall be as shown on the reverse side.




Fixed Ceiling Column (Select column size based on ceiling height)		
Model Number	Minimum Suggested Ceiling Height	Column Length "A"
CCF2-XX-YY	<input type="checkbox"/> 8'-0"	20"
	<input type="checkbox"/> 8'-6"	26"
	<input type="checkbox"/> 9'-0"	32"
	<input type="checkbox"/> 9'-6"	38"
	<input type="checkbox"/> 10'-0"	44"

#### NOTES:

- All dimensions are approximate and subject to change. Required installation dimensions are included in instructions supplied with the ceiling column.
- NFPA 99 2018 (5.1.5.17) states that where installed in a down-facing position, such as in a ceiling or ceiling columns, station outlets/inlets shall be DISS connectors.
- Rough-Ins can be shipped early on an as-needed basis. Contact the factory for further assistance.



#### Model Numbering Scheme

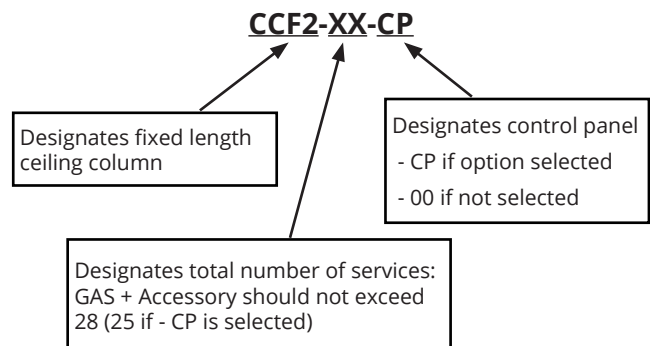

**Fixed Length Medical Ceiling Column**


Ceiling columns are manufactured to customer specifications. The drawing indicates the possible locations of services. Select the services desired and fill in the appropriate location, number or letter (A through P or 1 through 12) in the charts below. Multiple locations for a particular service may be selected.

Number of Columns \_\_\_\_\_ Column Length \_\_\_\_\_ Model Number \_\_\_\_\_

Project Name \_\_\_\_\_

Approved by \_\_\_\_\_ Date \_\_\_\_\_

Side 1 is assumed to be facing operating table



Control Panel <sup>5</sup> (Circle Gas Service and Side)					
Nitrogen	Instrument Air	Side 1	Side 2	Side 3	Side 4

**NOTES:**

1. BeaconMedaes requires a signed, approved copy of this specification before fabrication will begin.
2. NFPA 99 2018 (5.1.5.17) states that where installed in a down-facing position, such as in a ceiling or ceiling columns, station outlets/inlets shall be DISS connectors.
3. Blank cover plates are supplied for locations with a specified service.
4. Gases may only be located in 1-12 and D, H, L, P and no more than 12 per column.
5. No other services can be used on side of columns where control panels are used.
6. Electrical Services and other Accessories may only be used in locations A-P.
7. Electrical Services and other Accessories are not pre-installed on the column.
8. No conduit or wiring is provided on the fixed columns.

Gas Service	Outlet Type				Service Location(s) Indicate location(s) with letter or number	Quantity
	Geometric Index	Pin Index	Latch Key	DISS		
Oxygen						
Nitrous Oxide						
Air						
Vacuum						
WAGD						
Nitrogen	NOT AVAILABLE					
Instrument Air						
Carbon Dioxide						
He-O <sub>2</sub>						
O <sub>2</sub> -He						
CO <sub>2</sub> -O <sub>2</sub>						
O <sub>2</sub> -CO <sub>2</sub>						
<b>Accessory Services<sup>6</sup></b>						
Duplex Power Receptacle 125V, 20 AMP (Circle One Color)				Red		
				Ivory		
				Gray		
Duplex Power Receptacle 125V, 15 AMP (Circle One Color)				Red		
				Ivory		
				Gray		
Hubbellok® 23000HG Receptacle, 115V, 20 AMPS						
Future Electrical Provision						
Patient Monitoring Kit, Two 5 Pin Connectors						
I.V. Hooks						
RJ-45 Data Connection						
Vacuum Slide Bracket						
Grounding Receptacle						
<b>TOTAL SELECTED SERVICES (GAS + ACCESSORY)</b>						