

Note X:
 - Dimension drawing standardized
 - Air inlet flange details added
 - Mk-IV Elektronikon changed to Mk5

Ed	Posi- tion	See Note X	Gewijzigd van Modified from	2011-05-20 Datum Date	Ingev./Goedg. Intr./Appd.
03					

Approx. Mass ±110 (LBS)	
Type	Pack
ZR30	2535
ZR37	2646
ZR45	2694

Center of Gravity ±2 (inch)	
Dim.	Pack
W	20.3
L	38.0
H	23.9


All materials supplied are in compliance with the requirements of the List of Prohibited Substances


9820576900	02.11
Parent 3D model	Ed. - Version 3D

Tolerances, if not indicated, according to:				
ATLAS COPCO STANDARD CLASS				
Name	DIMENS.		ZR30-45 MED	Secrecy Class
Material	NOT APPLICABLE			1102 K / 3
Treatment	Not Applicable			INV
Scale	1:10	Family	A / Compare	Blank nr.
Drawn by	sraman	Blank nr.	Replaces	
Version Drwg	03.10	Blank wt.	0 Kg	Finl wt.
Des checked.		Prod checked.	Approved.	Date
				2008-01-22
Approved		9820576900		


Note:
 * With full open door




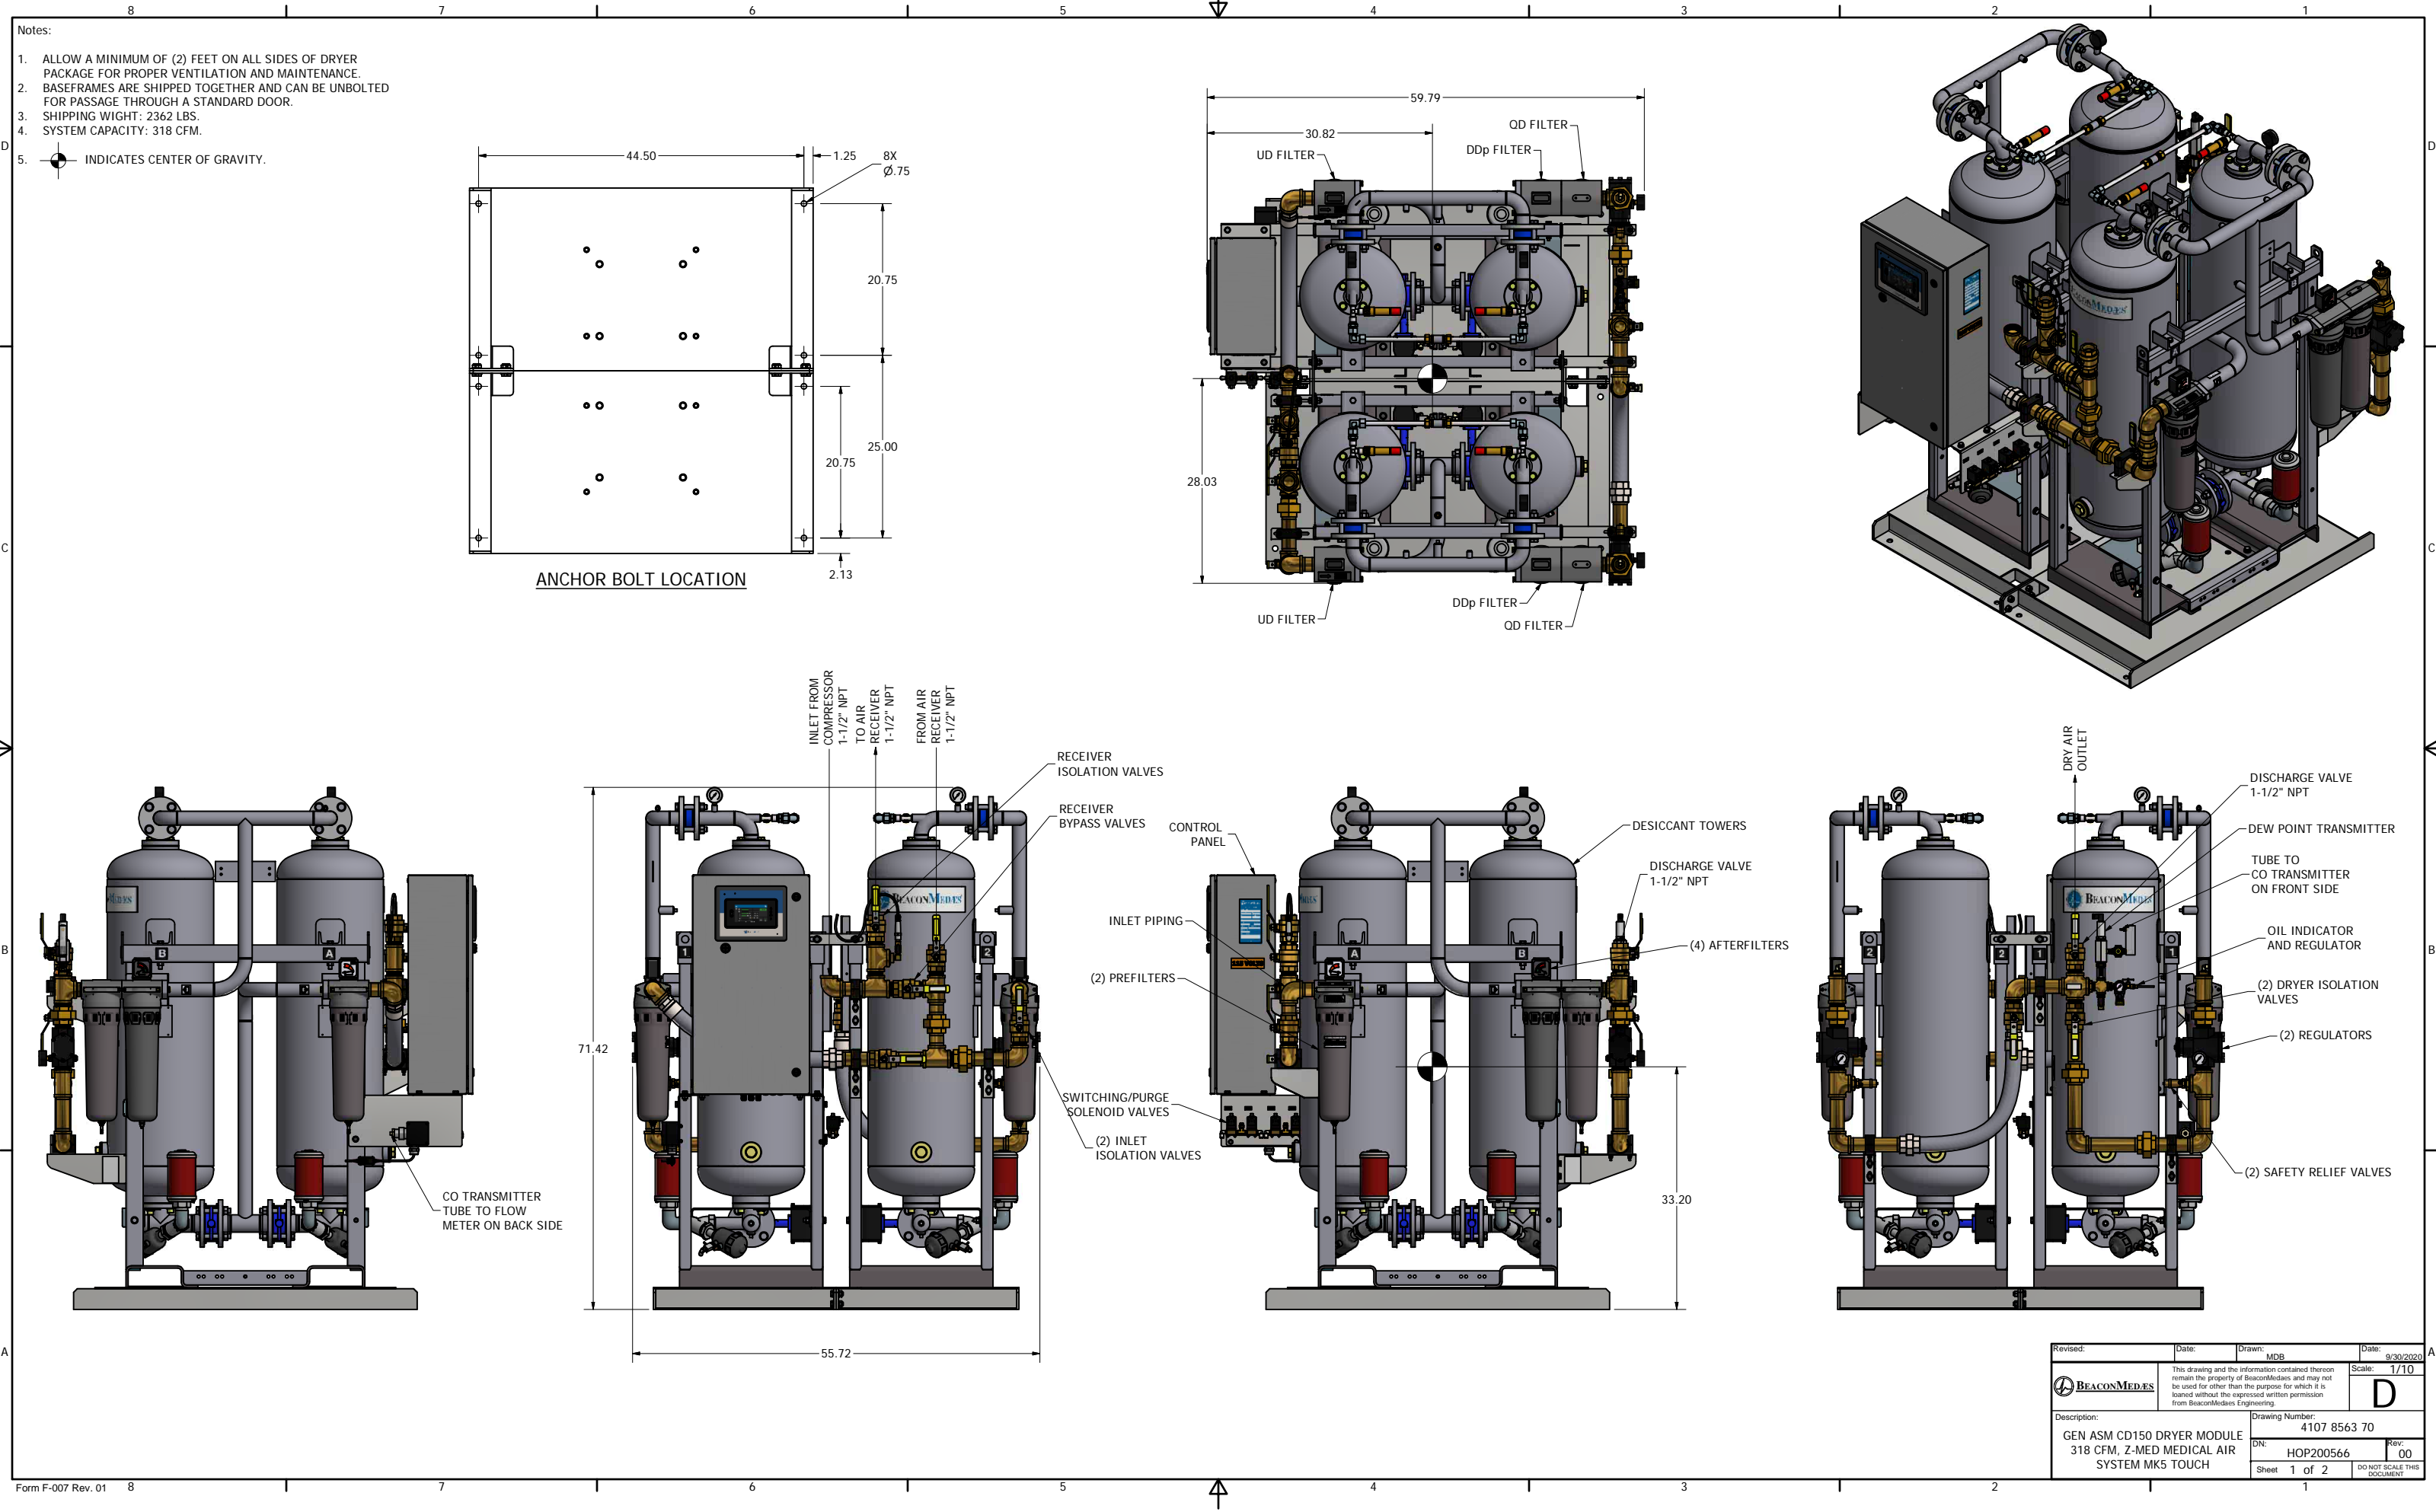

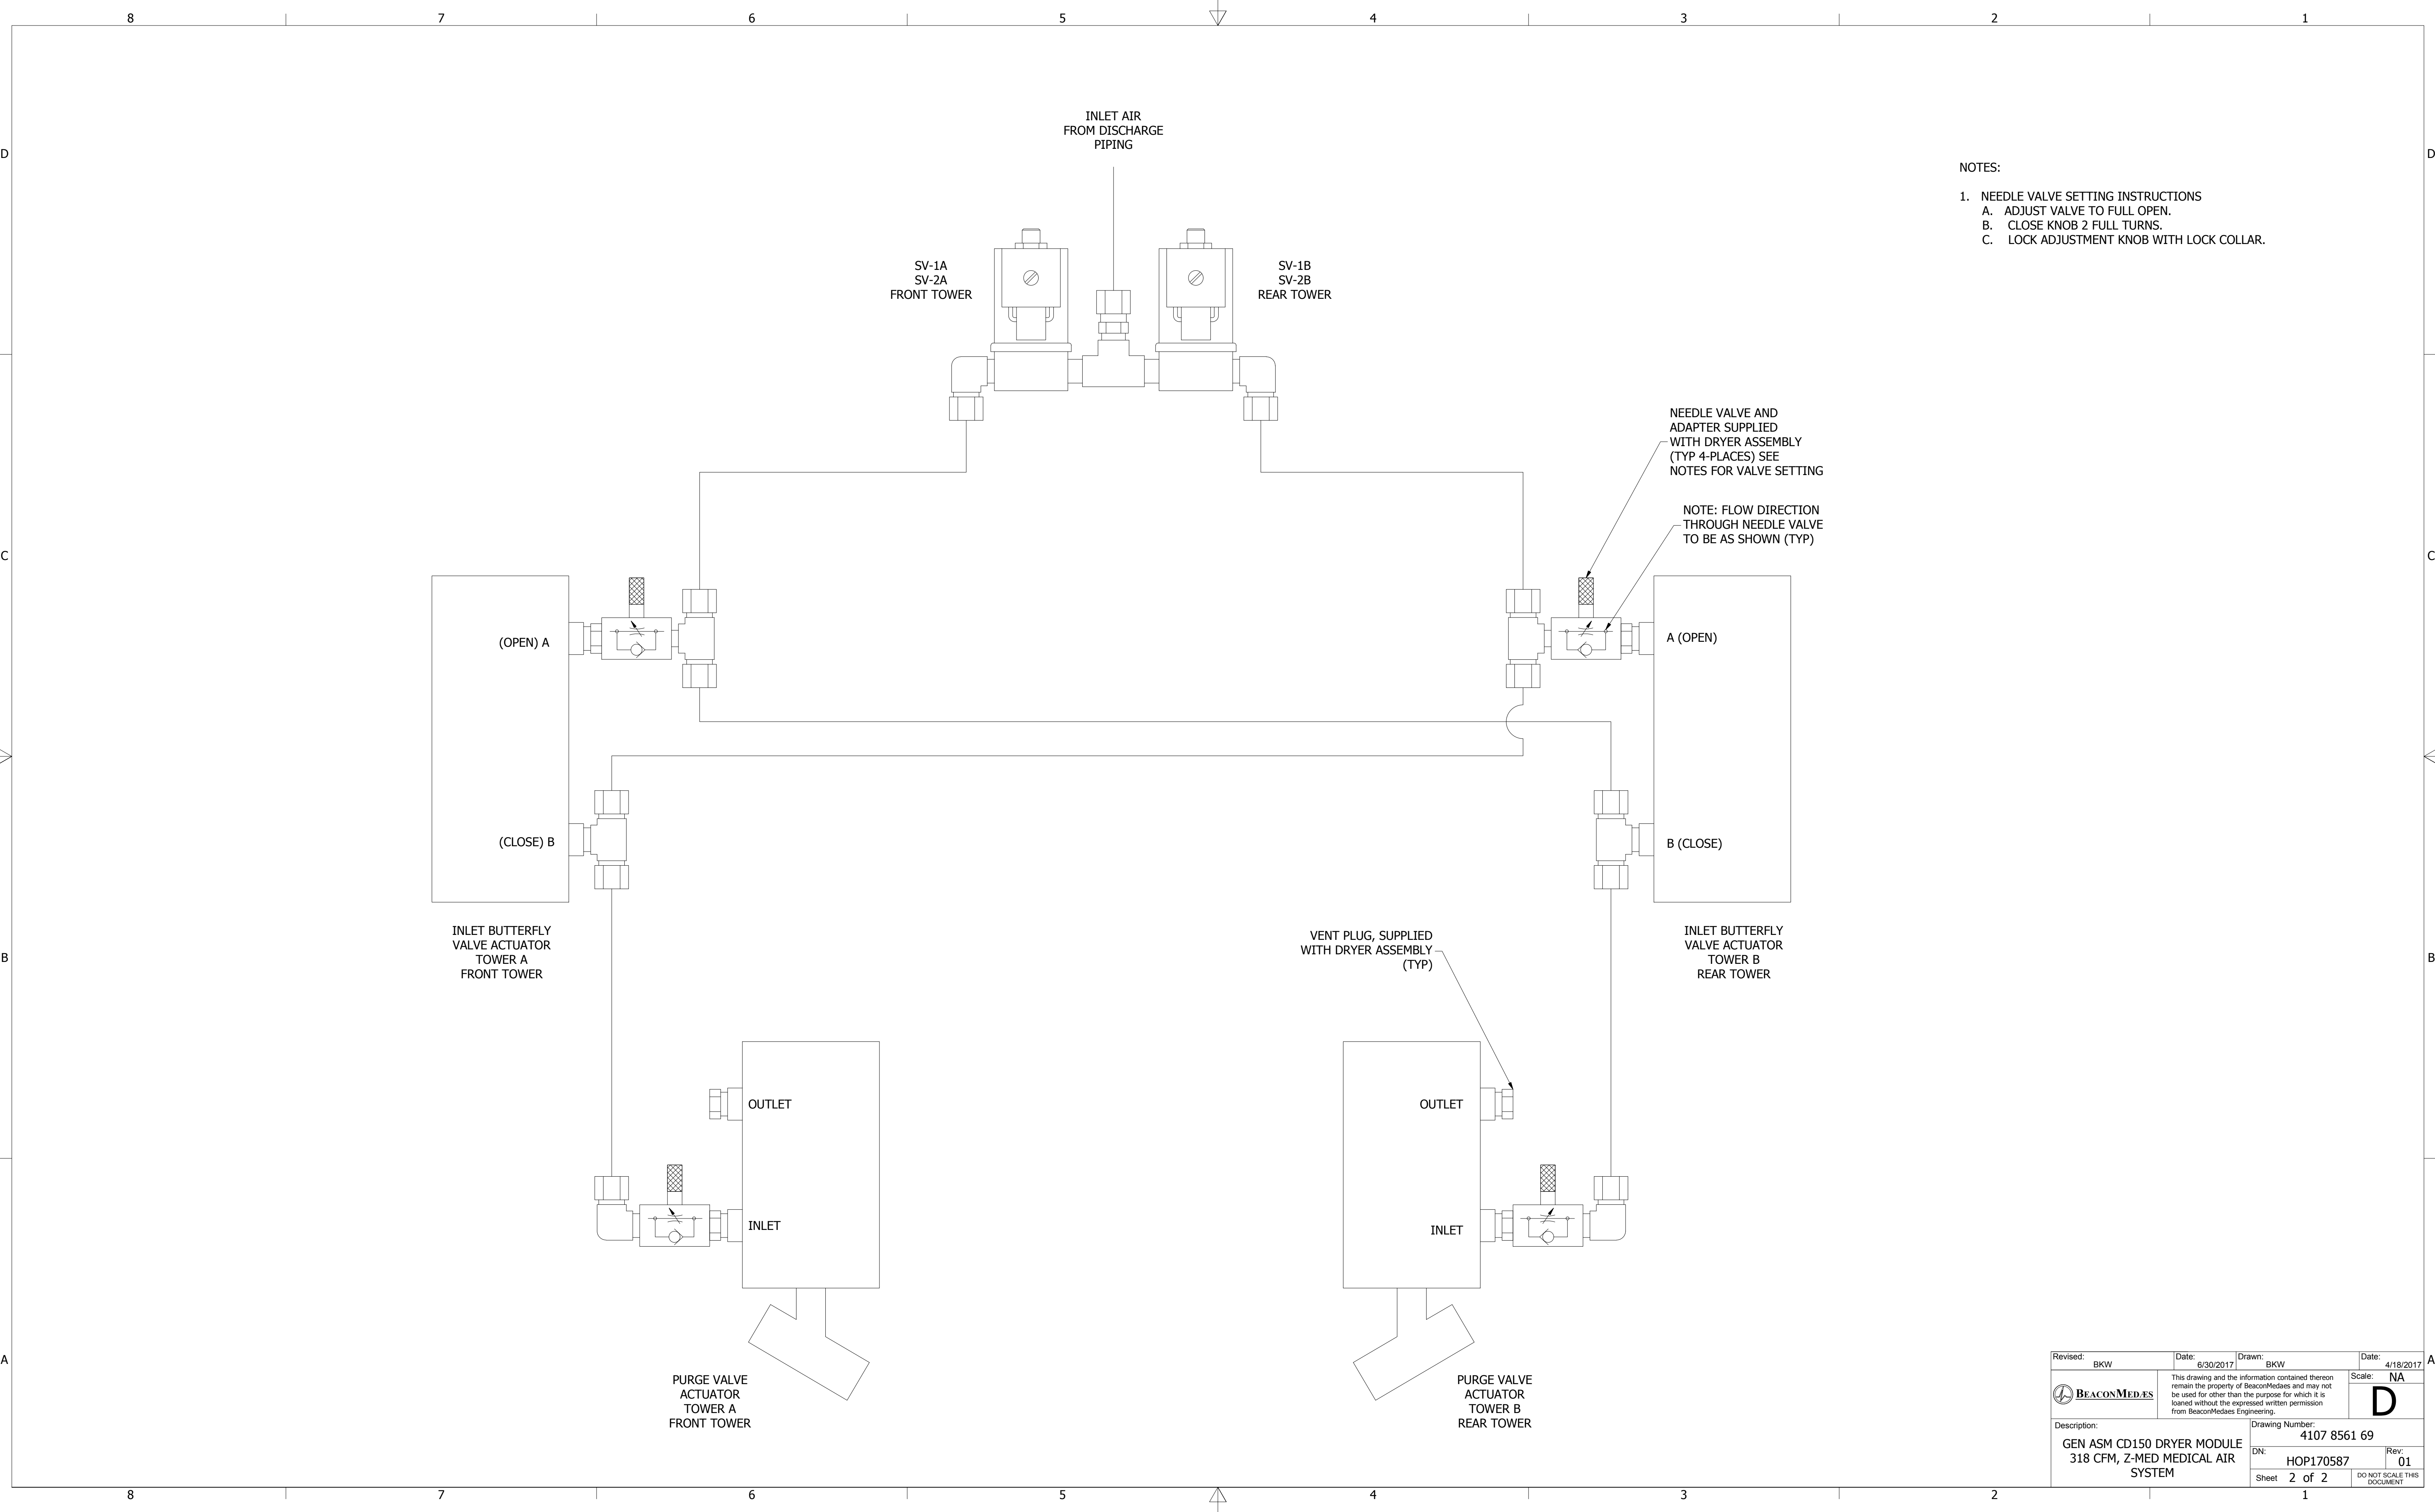

- NOTES:
- NEEDLE VALVE SETTING INSTRUCTIONS
 - ADJUST VALVE TO FULL OPEN.
 - CLOSE KNOB 2 FULL TURNS.
 - LOCK ADJUSTMENT KNOB WITH LOCK COLLAR.

Revised: BKW	Date: 6/30/2017	Drawn: BKW	Date: 4/18/2017
 BEACONMEDAES	This drawing and the information contained therein remain the property of BeaconMedaes and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedaes Engineering.		Scale: NA
Description: GEN ASM CD150 DRYER MODULE 318 CFM, Z-MED MEDICAL AIR SYSTEM		Drawing Number: 4107 8561 69	
DN: HOP170587		Rev: 01	
Sheet 2 of 2		DO NOT SCALE THIS DOCUMENT	

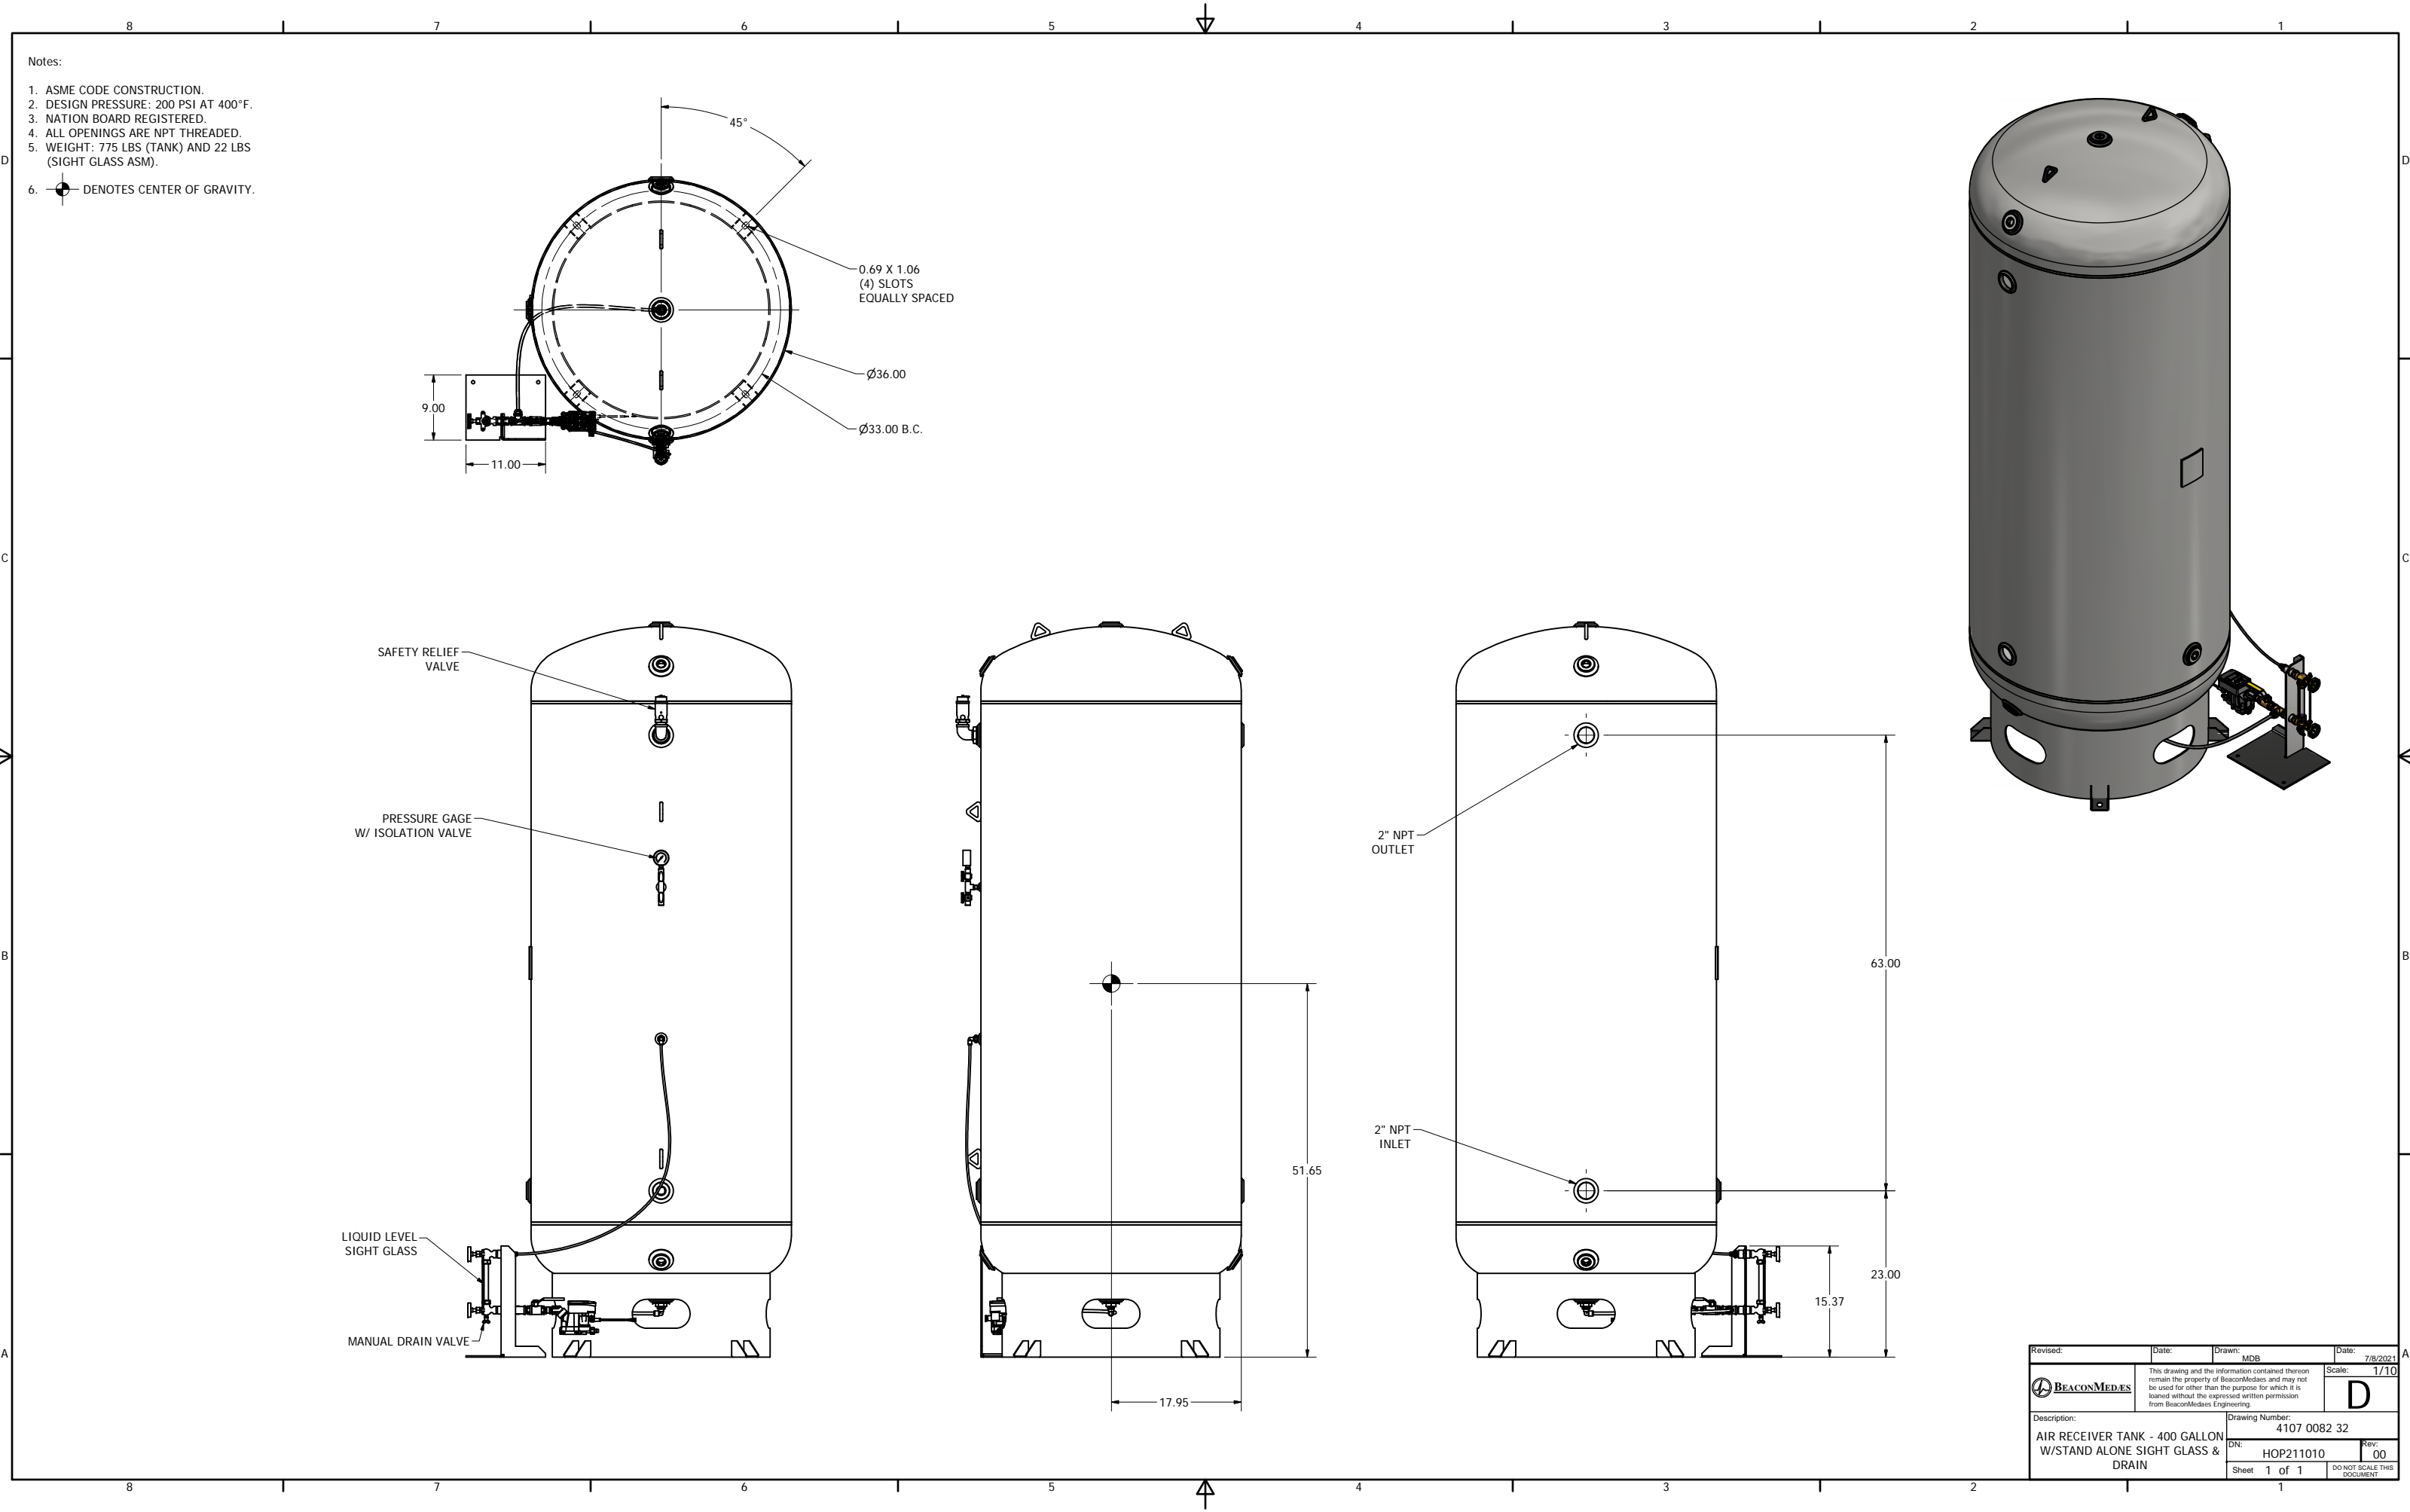

Revised:	Date:	Drawn: MDB	Date: 7/8/2021
BEACONMEDES	This drawing and the information contained therein remain the property of BeaconMedes and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedes Engineering.		Scale: 1/10
Description: AIR RECEIVER TANK - 400 GALLON W/STAND ALONE SIGHT GLASS & DRAIN		Drawing Number: 4107 0082 32	Rev: 00
Sheet 1 of 1		DN: HOP211010	DO NOT SCALE THIS DOCUMENT