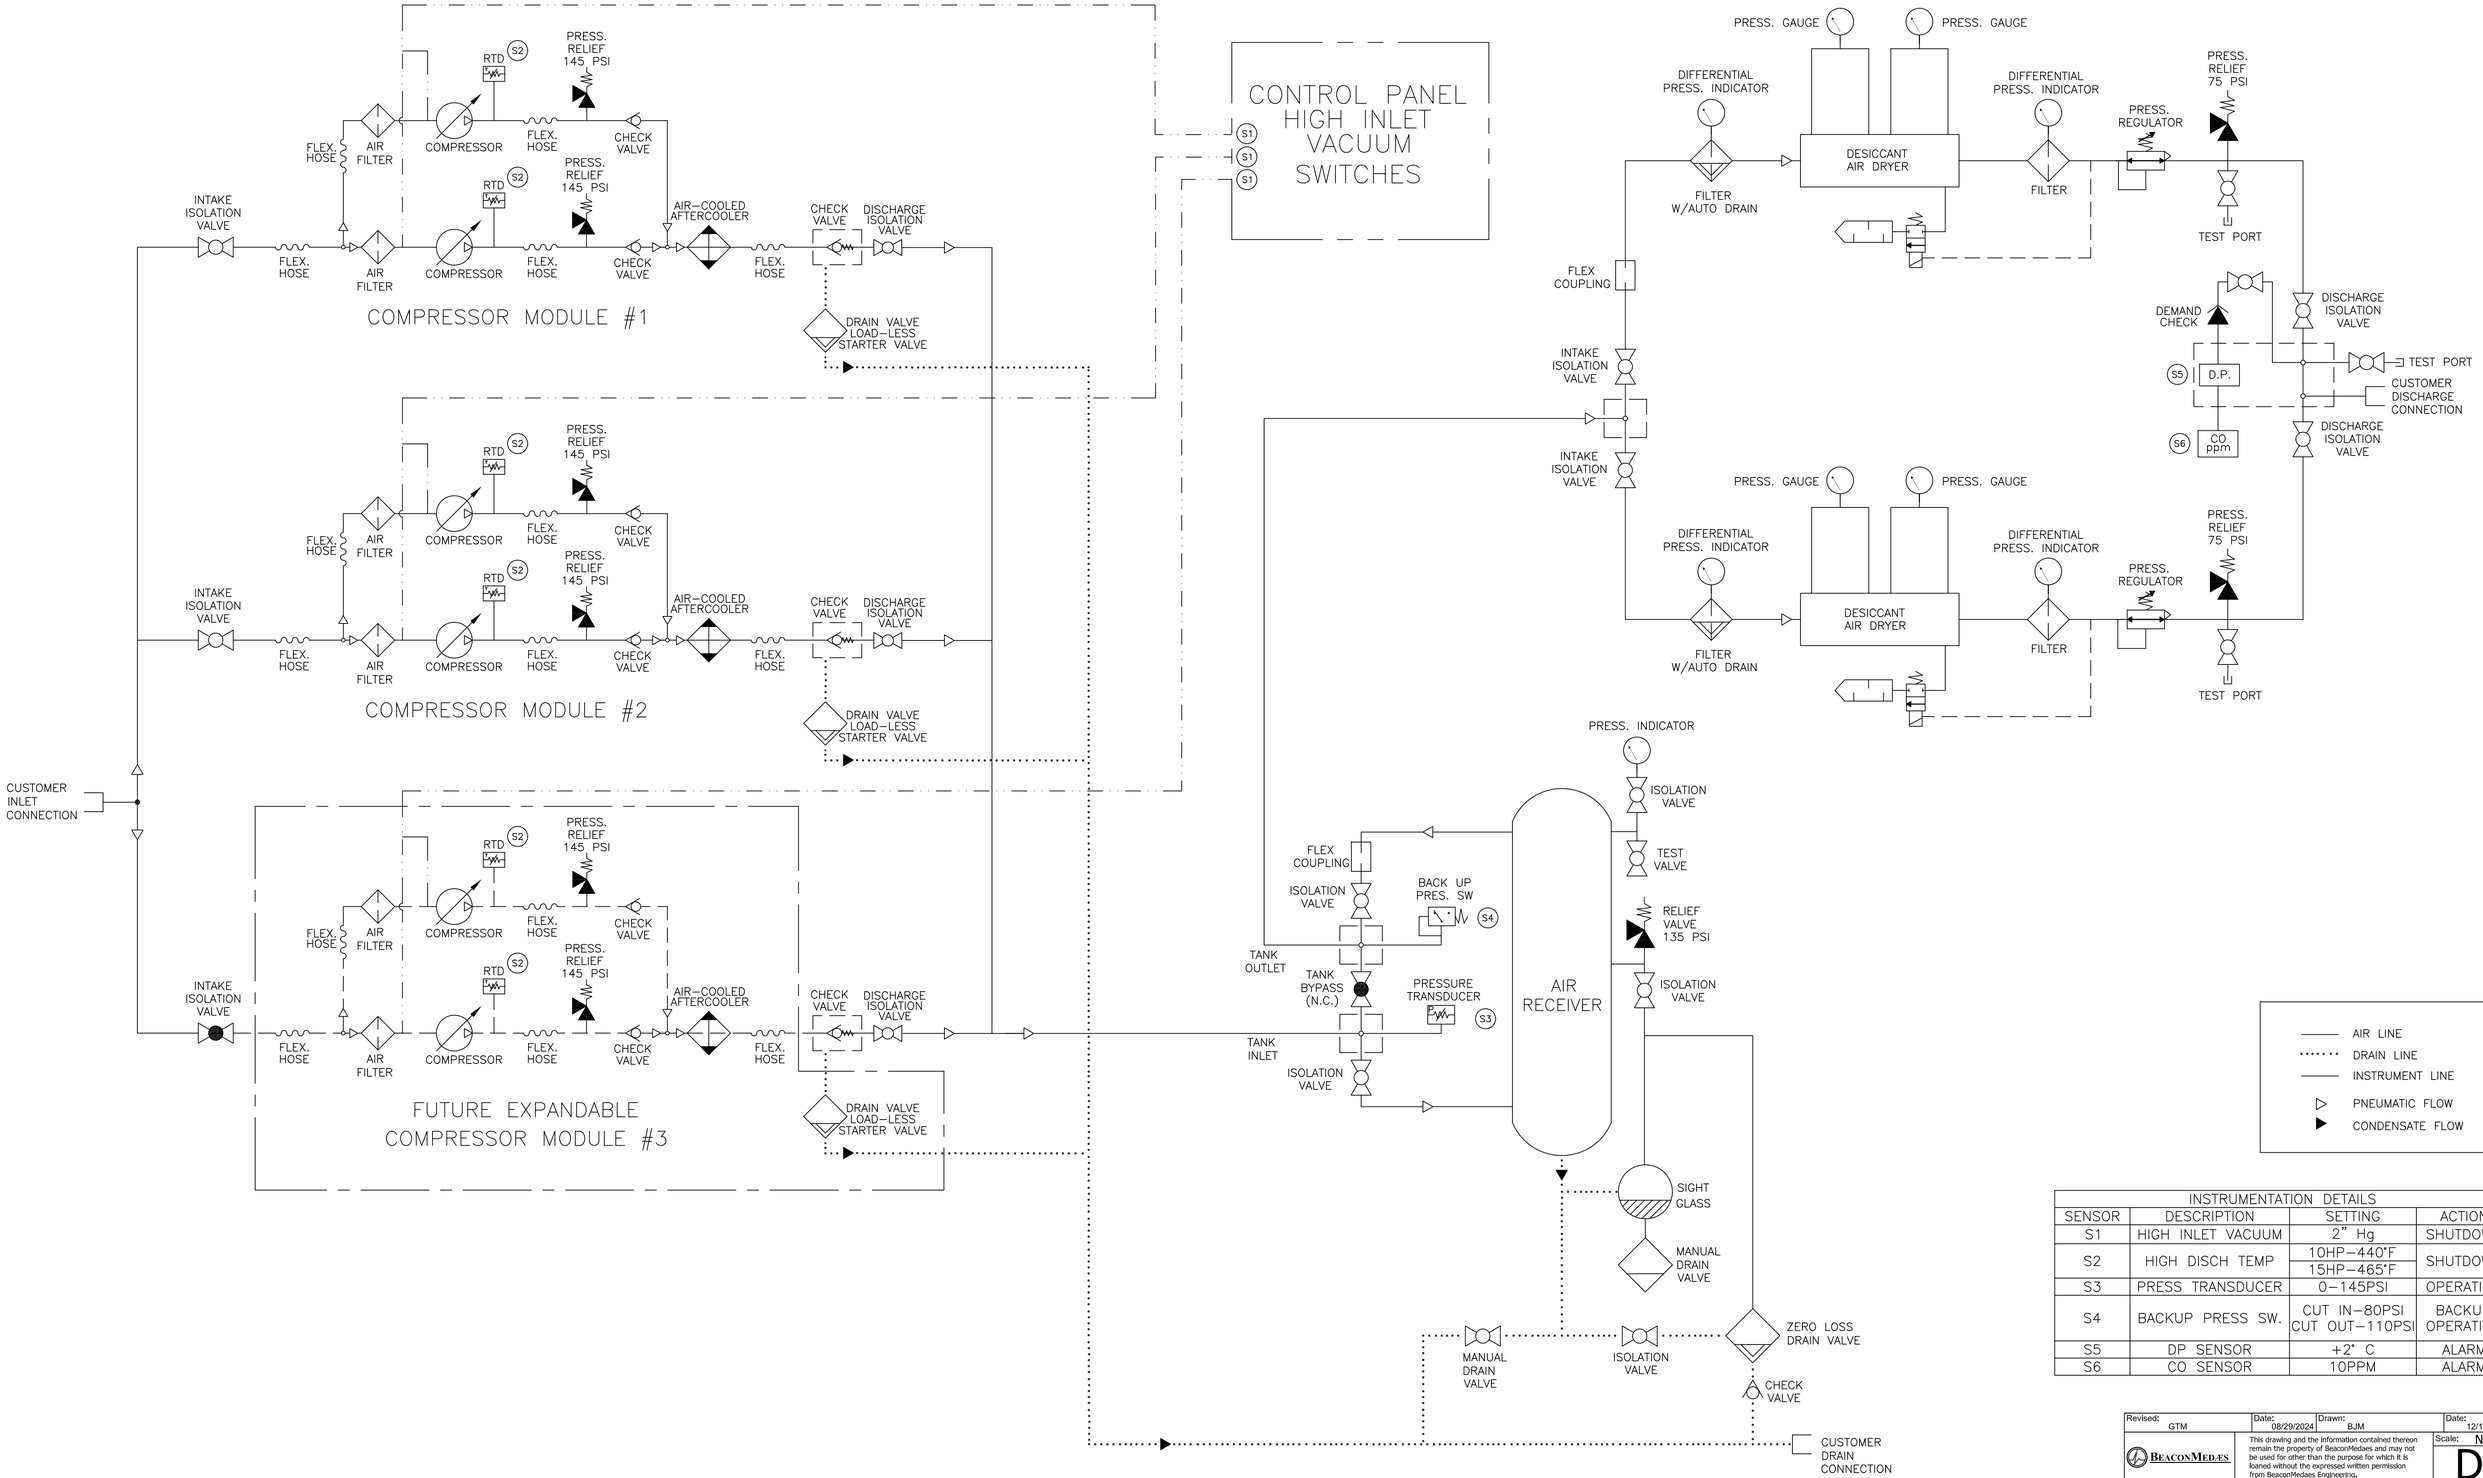


| INSTRUMENTATION DETAILS | | | |
|---|---|---|---|
| SENSOR | DESCRIPTION | SETTING | ACTION |
| S1 | HIGH INLET VACUUM | 2" Hg | SHUTDOWN |
| S2 | HIGH DISCH TEMP | 10HP–440°F | SHUTDOWN |
| | | 15HP–465°F | |
| S3 | PRESS TRANSDUCER | 0–145PSI | OPERATION |
| S4 | BACKUP PRESS SW. | CUT IN–80PSI<br>CUT OUT–110PSI | BACKUP OPERATION |
| S5 | DP SENSOR | +2° C | ALARM |
| S6 | CO SENSOR | 10PPM | ALARM |

| | | | |
|---|---|---|---|
| Revised: GTM | Date: 08/29/2024 | Drawn: BJM | Date: 12/16/2009 |
| BeaconMed∧s | This drawing and the information contained thereon remain the property of BeaconMedaes and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedaes Engineering. | | Scale: NTS<br>D |
| Description: PNEUMATIC DIAGRAM DX-EXP-TX SCROLL SPC W/DRYER (10-15HP) | | Part Number: 4107 8512 07 | |
| | | DN: HOP240470 | Rev: 02 |
| | | Sheet 1 of 1 | DO NOT SCALE THIS DOCUMENT |