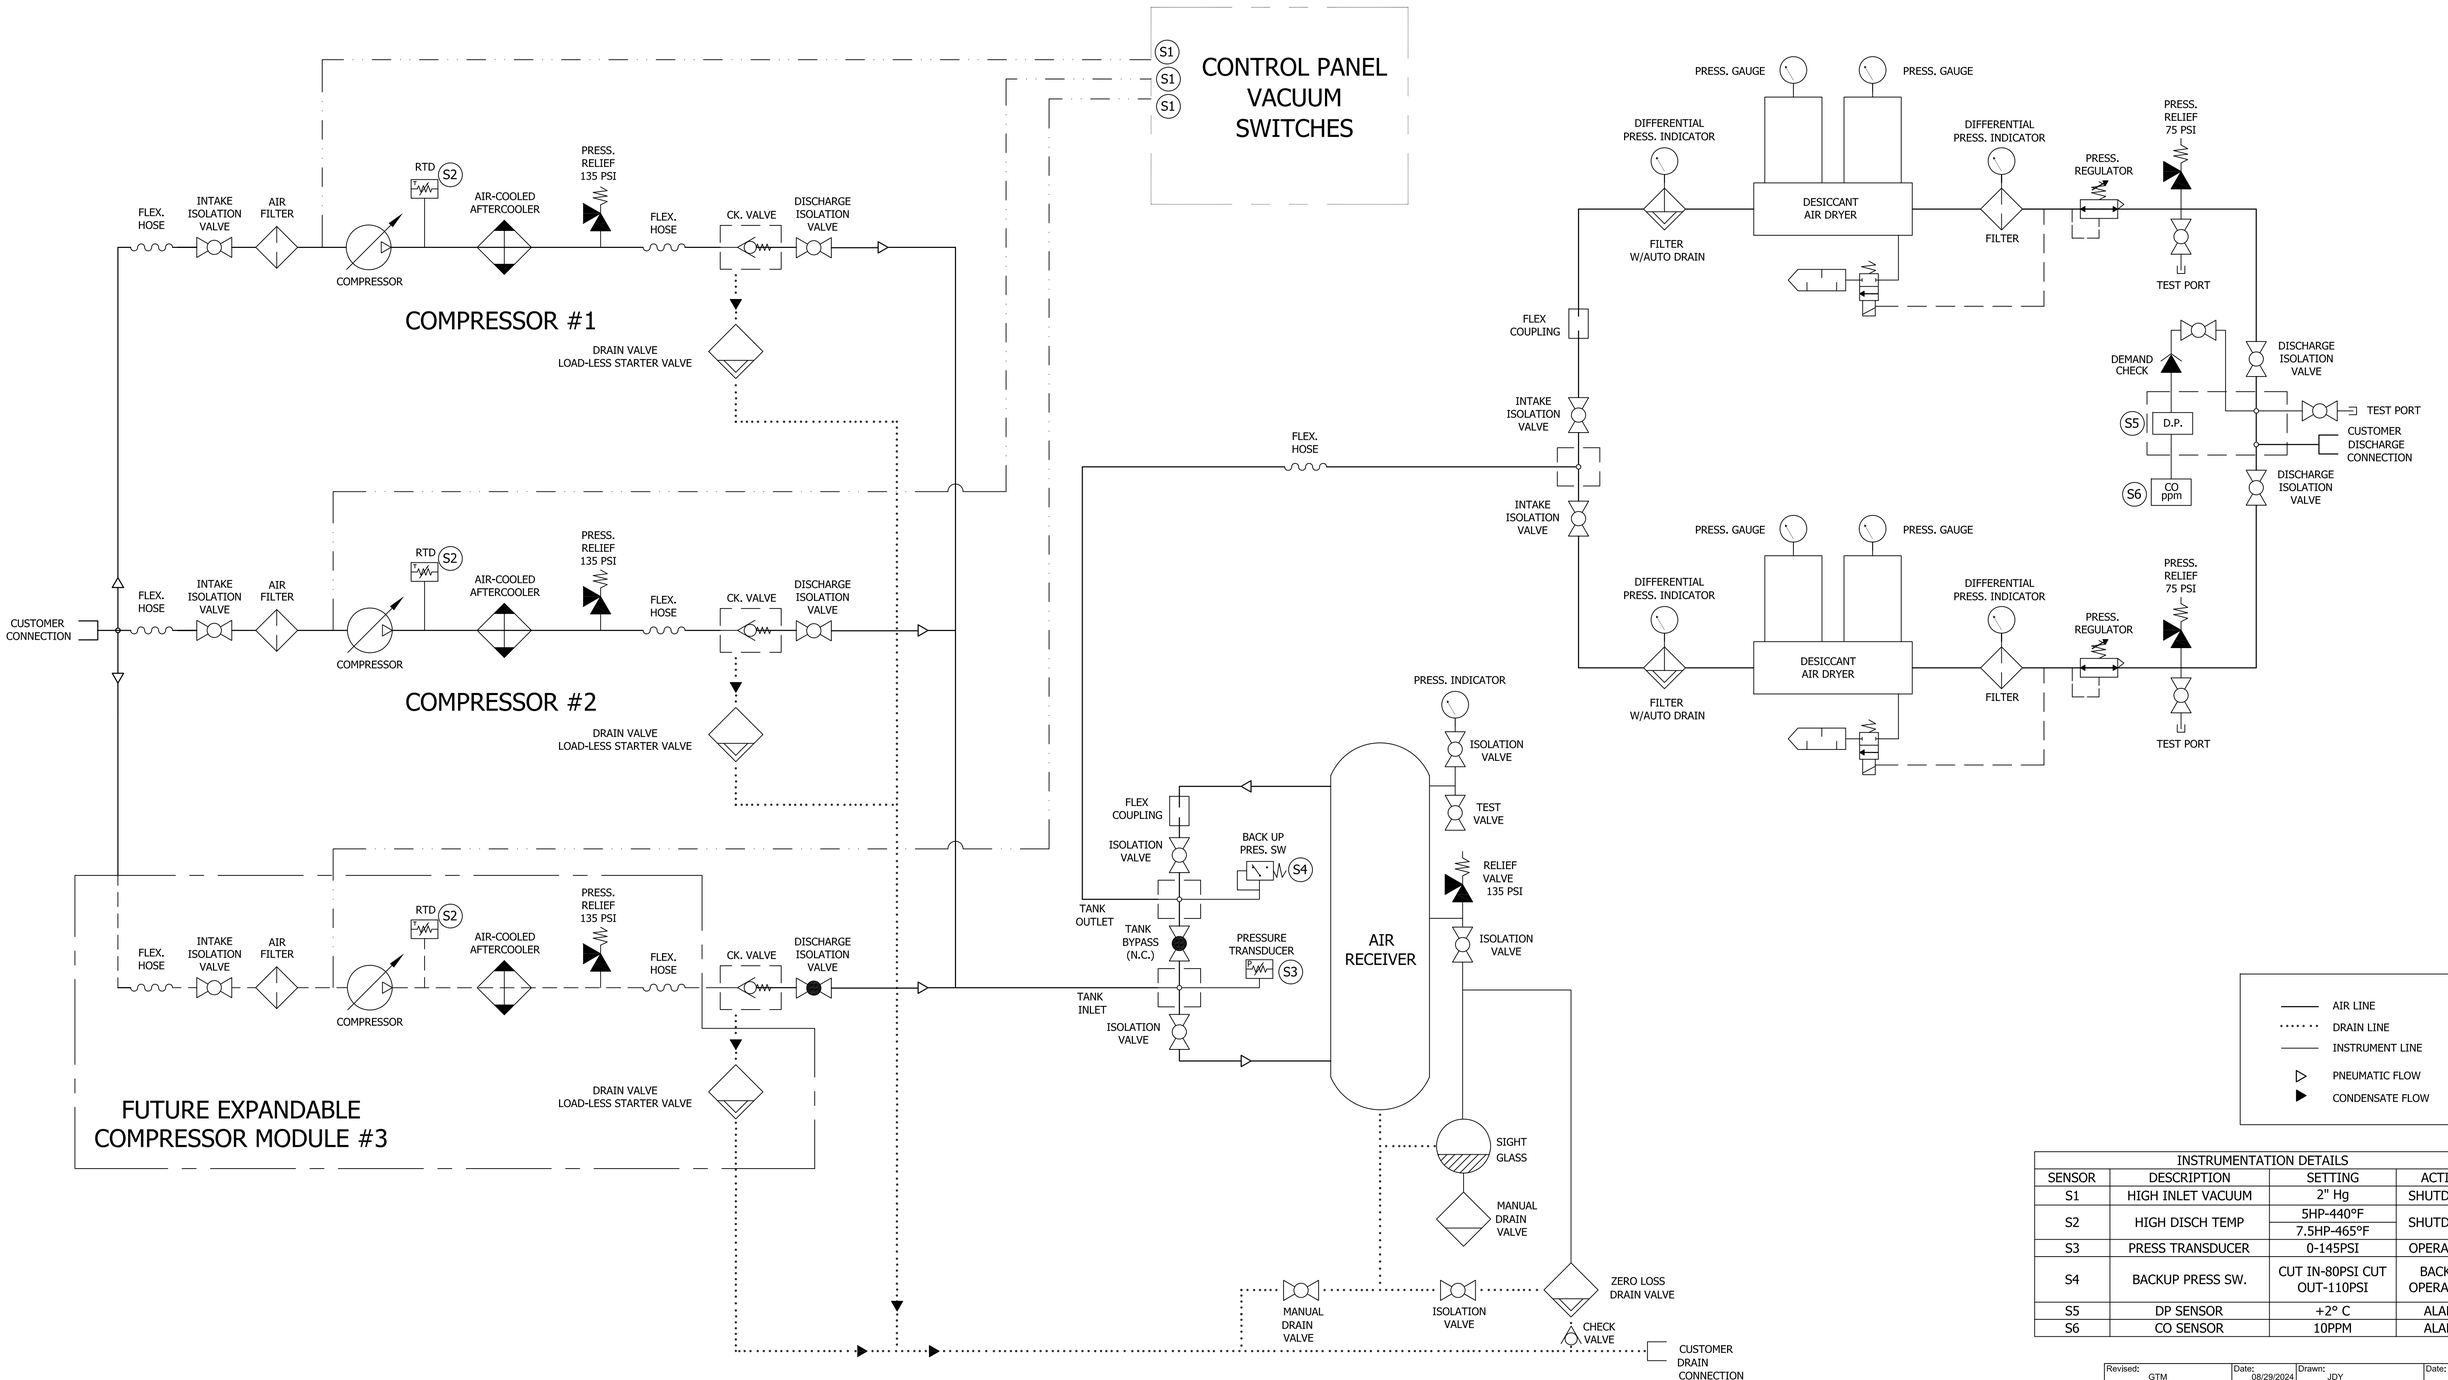

INSTRUMENTATION DETAILS			
SENSOR	DESCRIPTION	SETTING	ACTION
S1	HIGH INLET VACUUM	2" Hg	SHUTDOWN
S2	HIGH DISCH TEMP	5HP-440°F	SHUTDOWN
		7.5HP-465°F	
S3	PRESS TRANSDUCER	0-145PSI	OPERATION
S4	BACKUP PRESS SW.	CUT IN-80PSI CUT OUT-110PSI	BACKUP OPERATION
S5	DP SENSOR	+2° C	ALARM
S6	CO SENSOR	10PPM	ALARM

Revised: GTM	Date: 08/29/2024	Drawn: JDY	Date: 3/29/2010
BeaconMedæs	This drawing and the information contained thereon remain the property of BeaconMedaes and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedaes Engineering.		Scale: NTS
			D
Description: PNEUMATIC DIAGRAM DX-EXP-TX SCROLL SPC W/DRYER (5-7.5HP)		Part Number: 4107 8519 27	
		DN: HOP240470	Rev: 02
		Sheet 1 of 1	DO NOT SCALE THIS DOCUMENT