

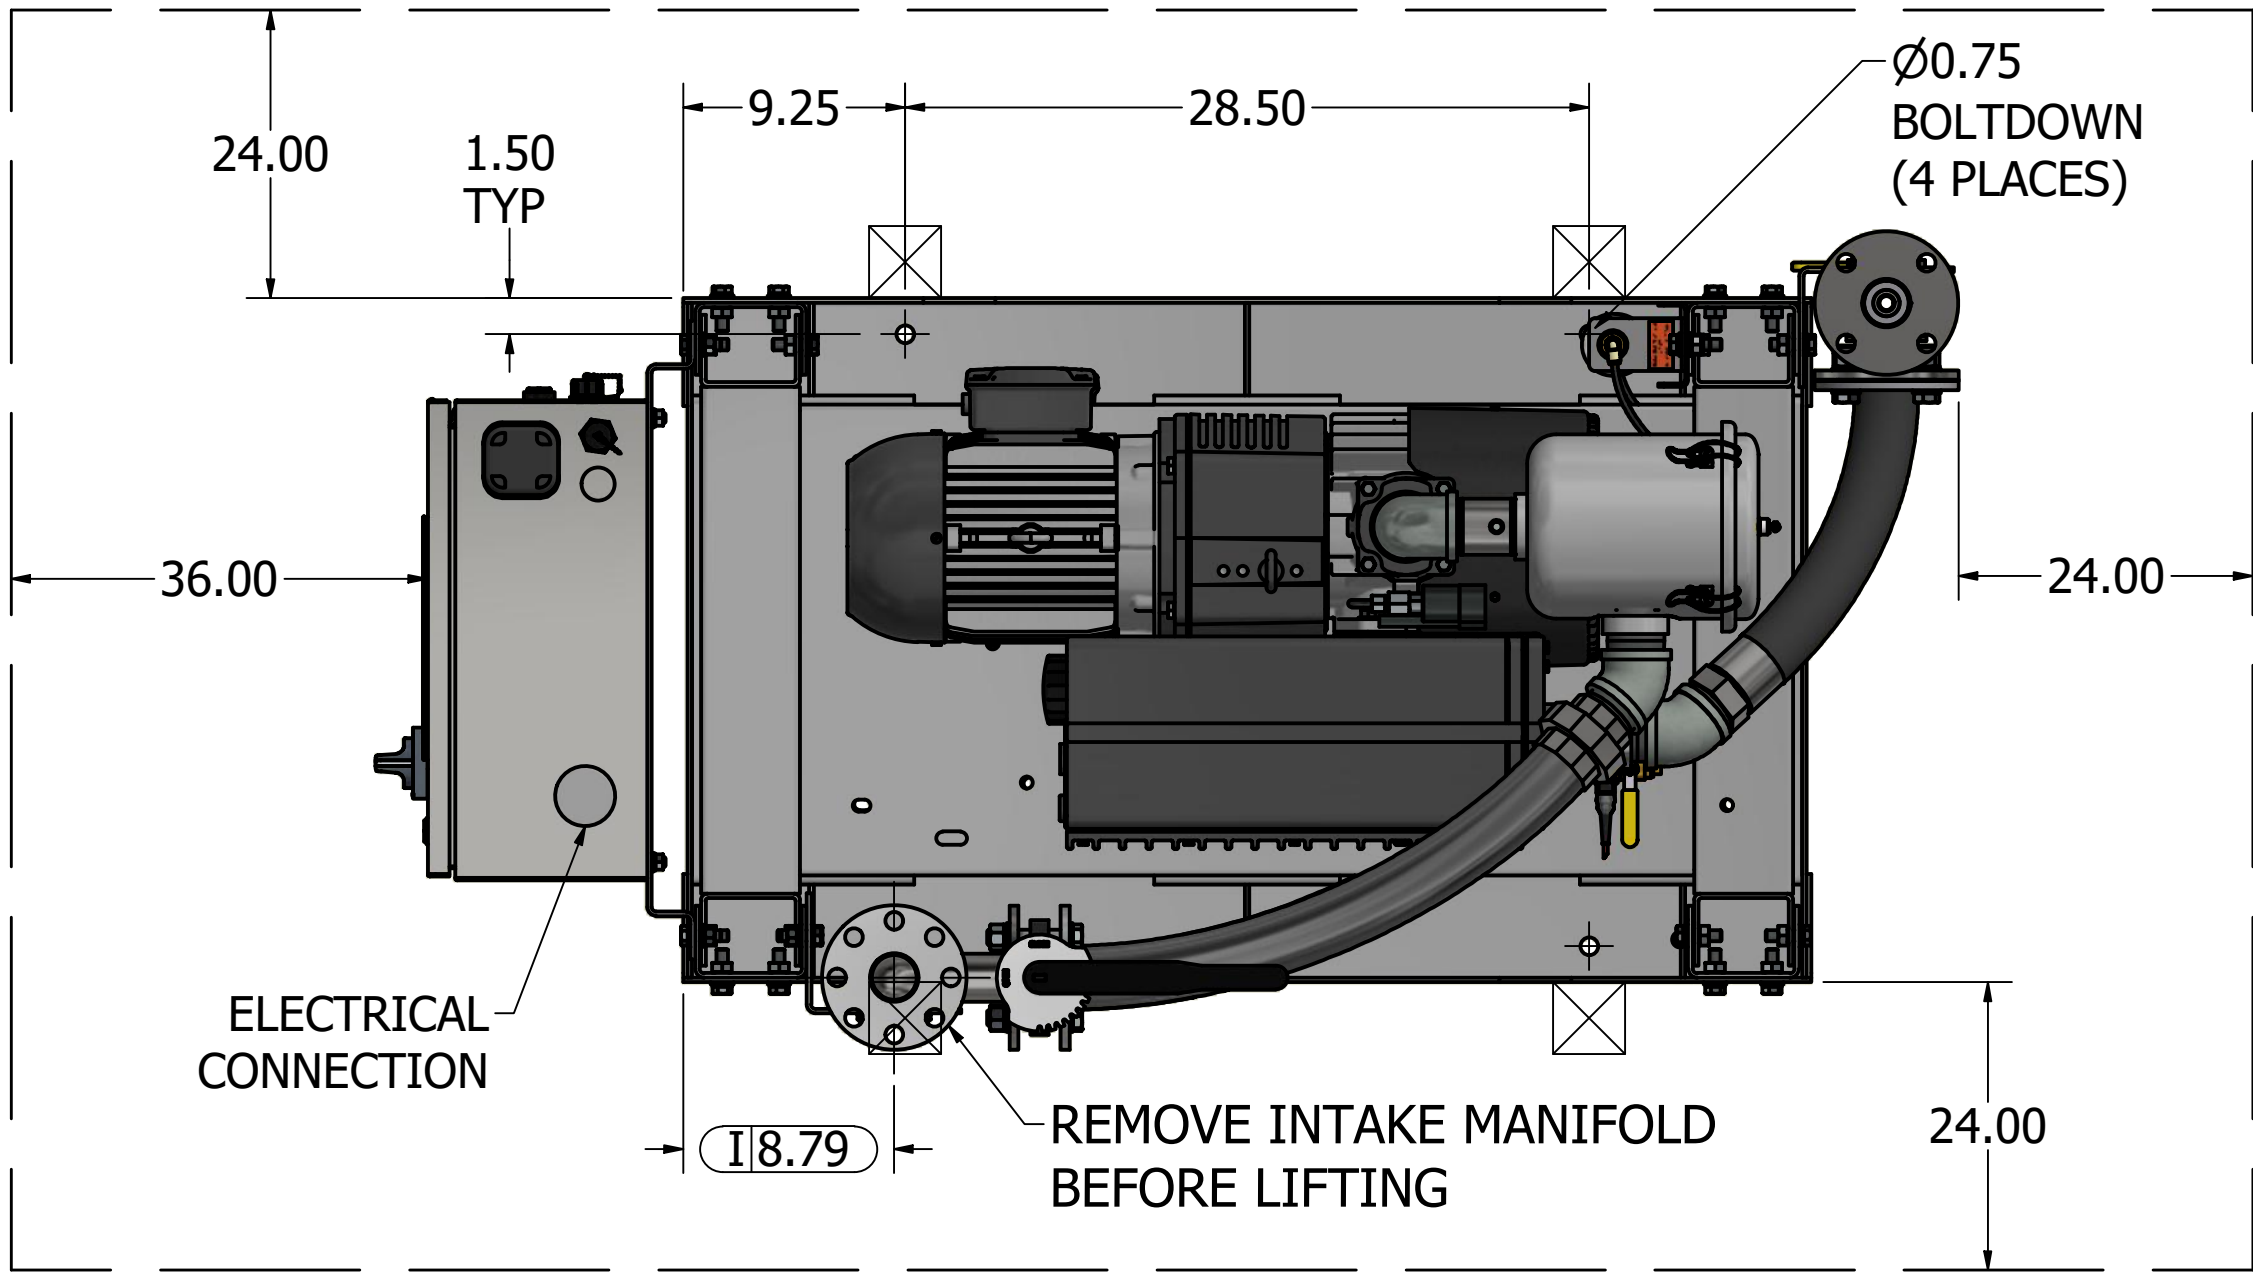


Notes:

1. DX MODULE WEIGHT: 1,045 LBS
240G TANK WEIGHT: 693 LBS
3.  INDICATES LIFTING POINT.
4.  DENOTES CENTER OF GRAVITY.

SYSTEM CONNECTIONS	
ID	DESCRIPTION
I	INLET LOCATION
D	DISCHARGE LOCATION
C	CONDENSATE DRAIN LOCATION
T	TANK DRAIN



MINIMUM CLEARANCE FOR
MAINTENANCE & VENTILATION


OUTLET
2" FLANGE

RECEIVER BYPASS
VALVE




HOSPITAL CONN
2" FLANGE


MANUAL DRAIN CONN.
1/2" NPT (FEMALE)

0.56 X 0.88 SLOT
Ø26.00 B.C.
EQUALLY SPACED
(4 PLACES)

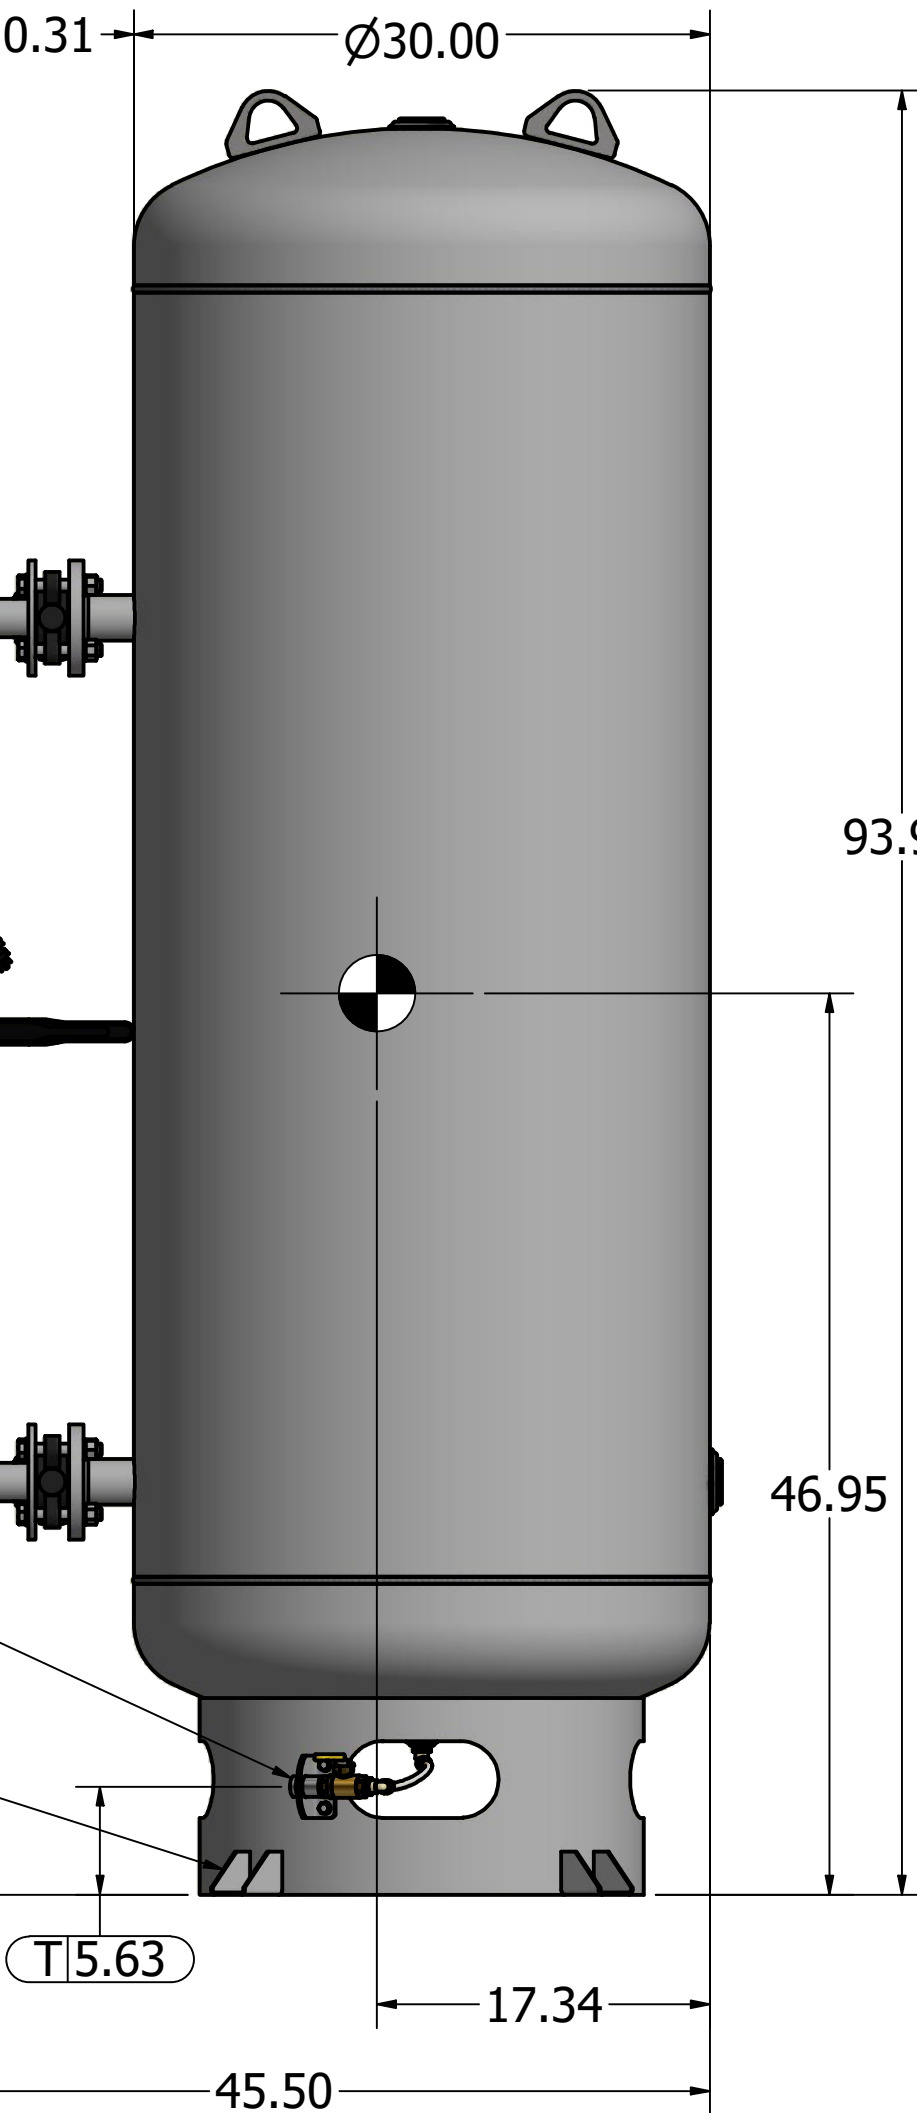

240 GAL VACUUM RECEIVER
2" FLANGED CONNECTIONS
(SCALE 1:10)

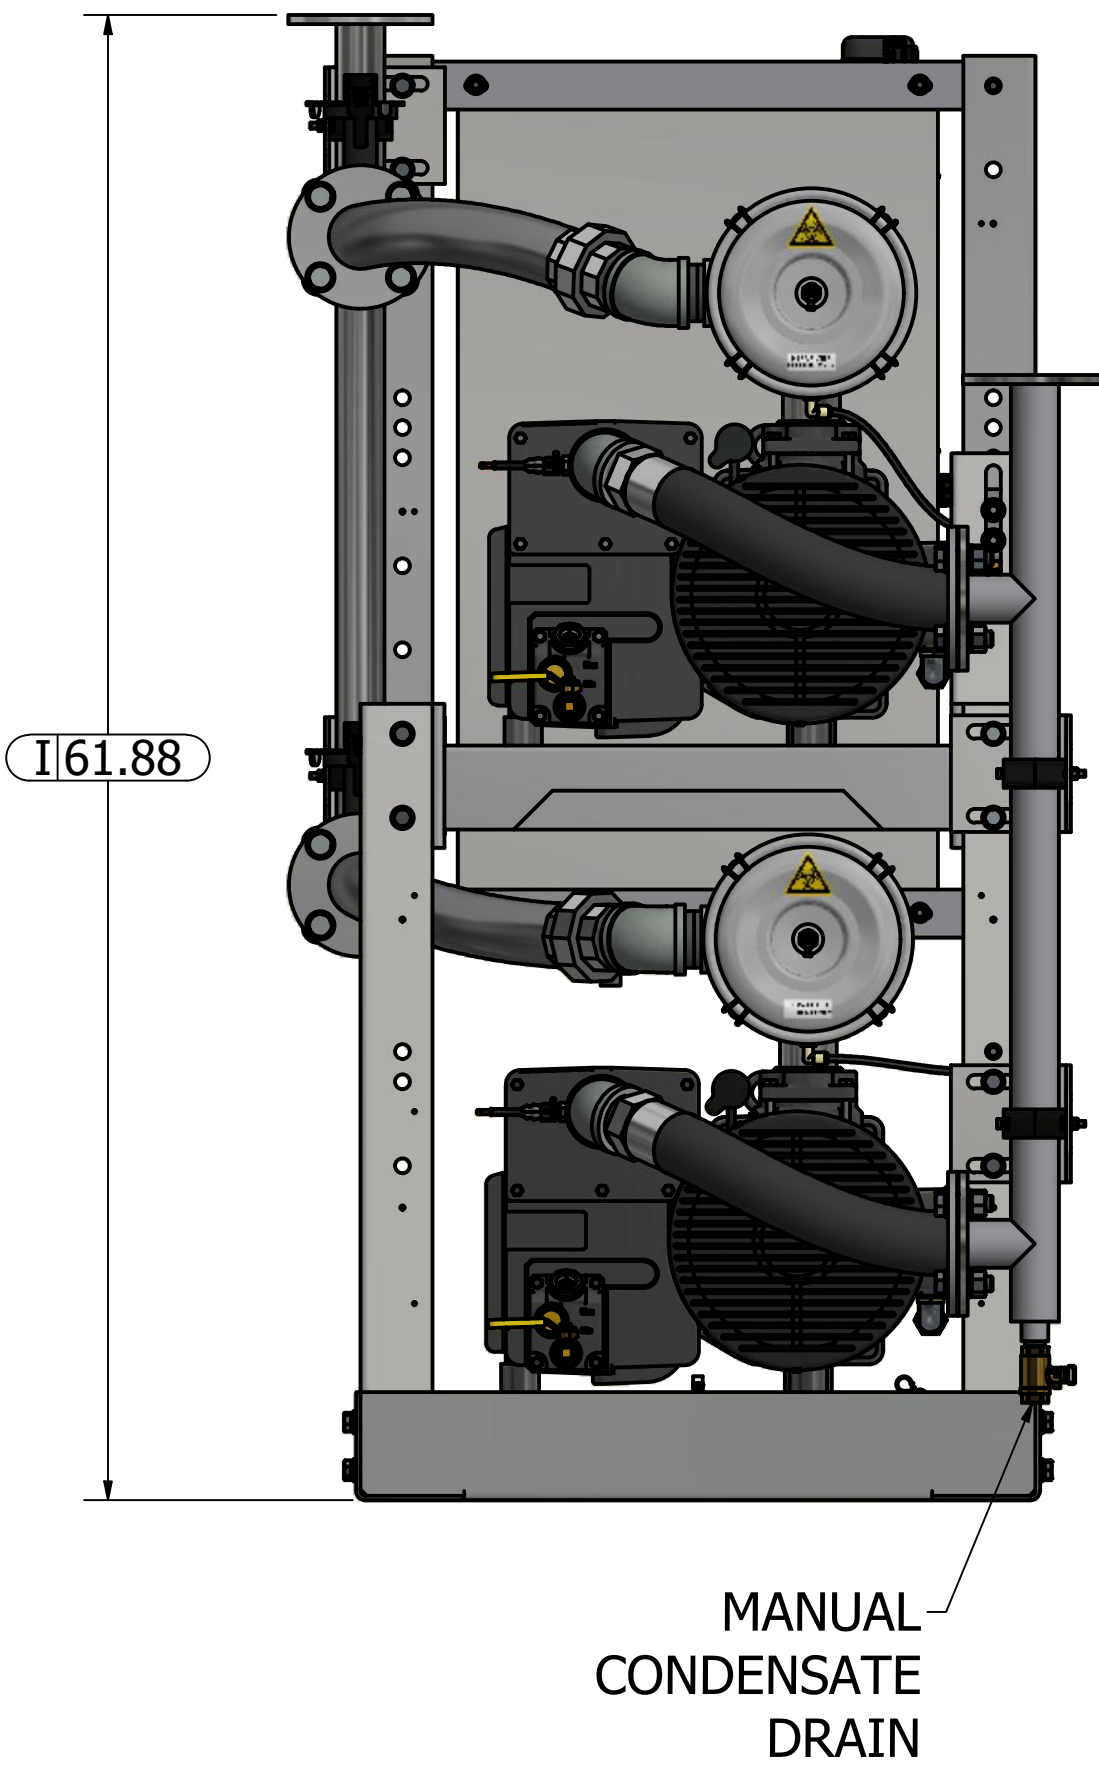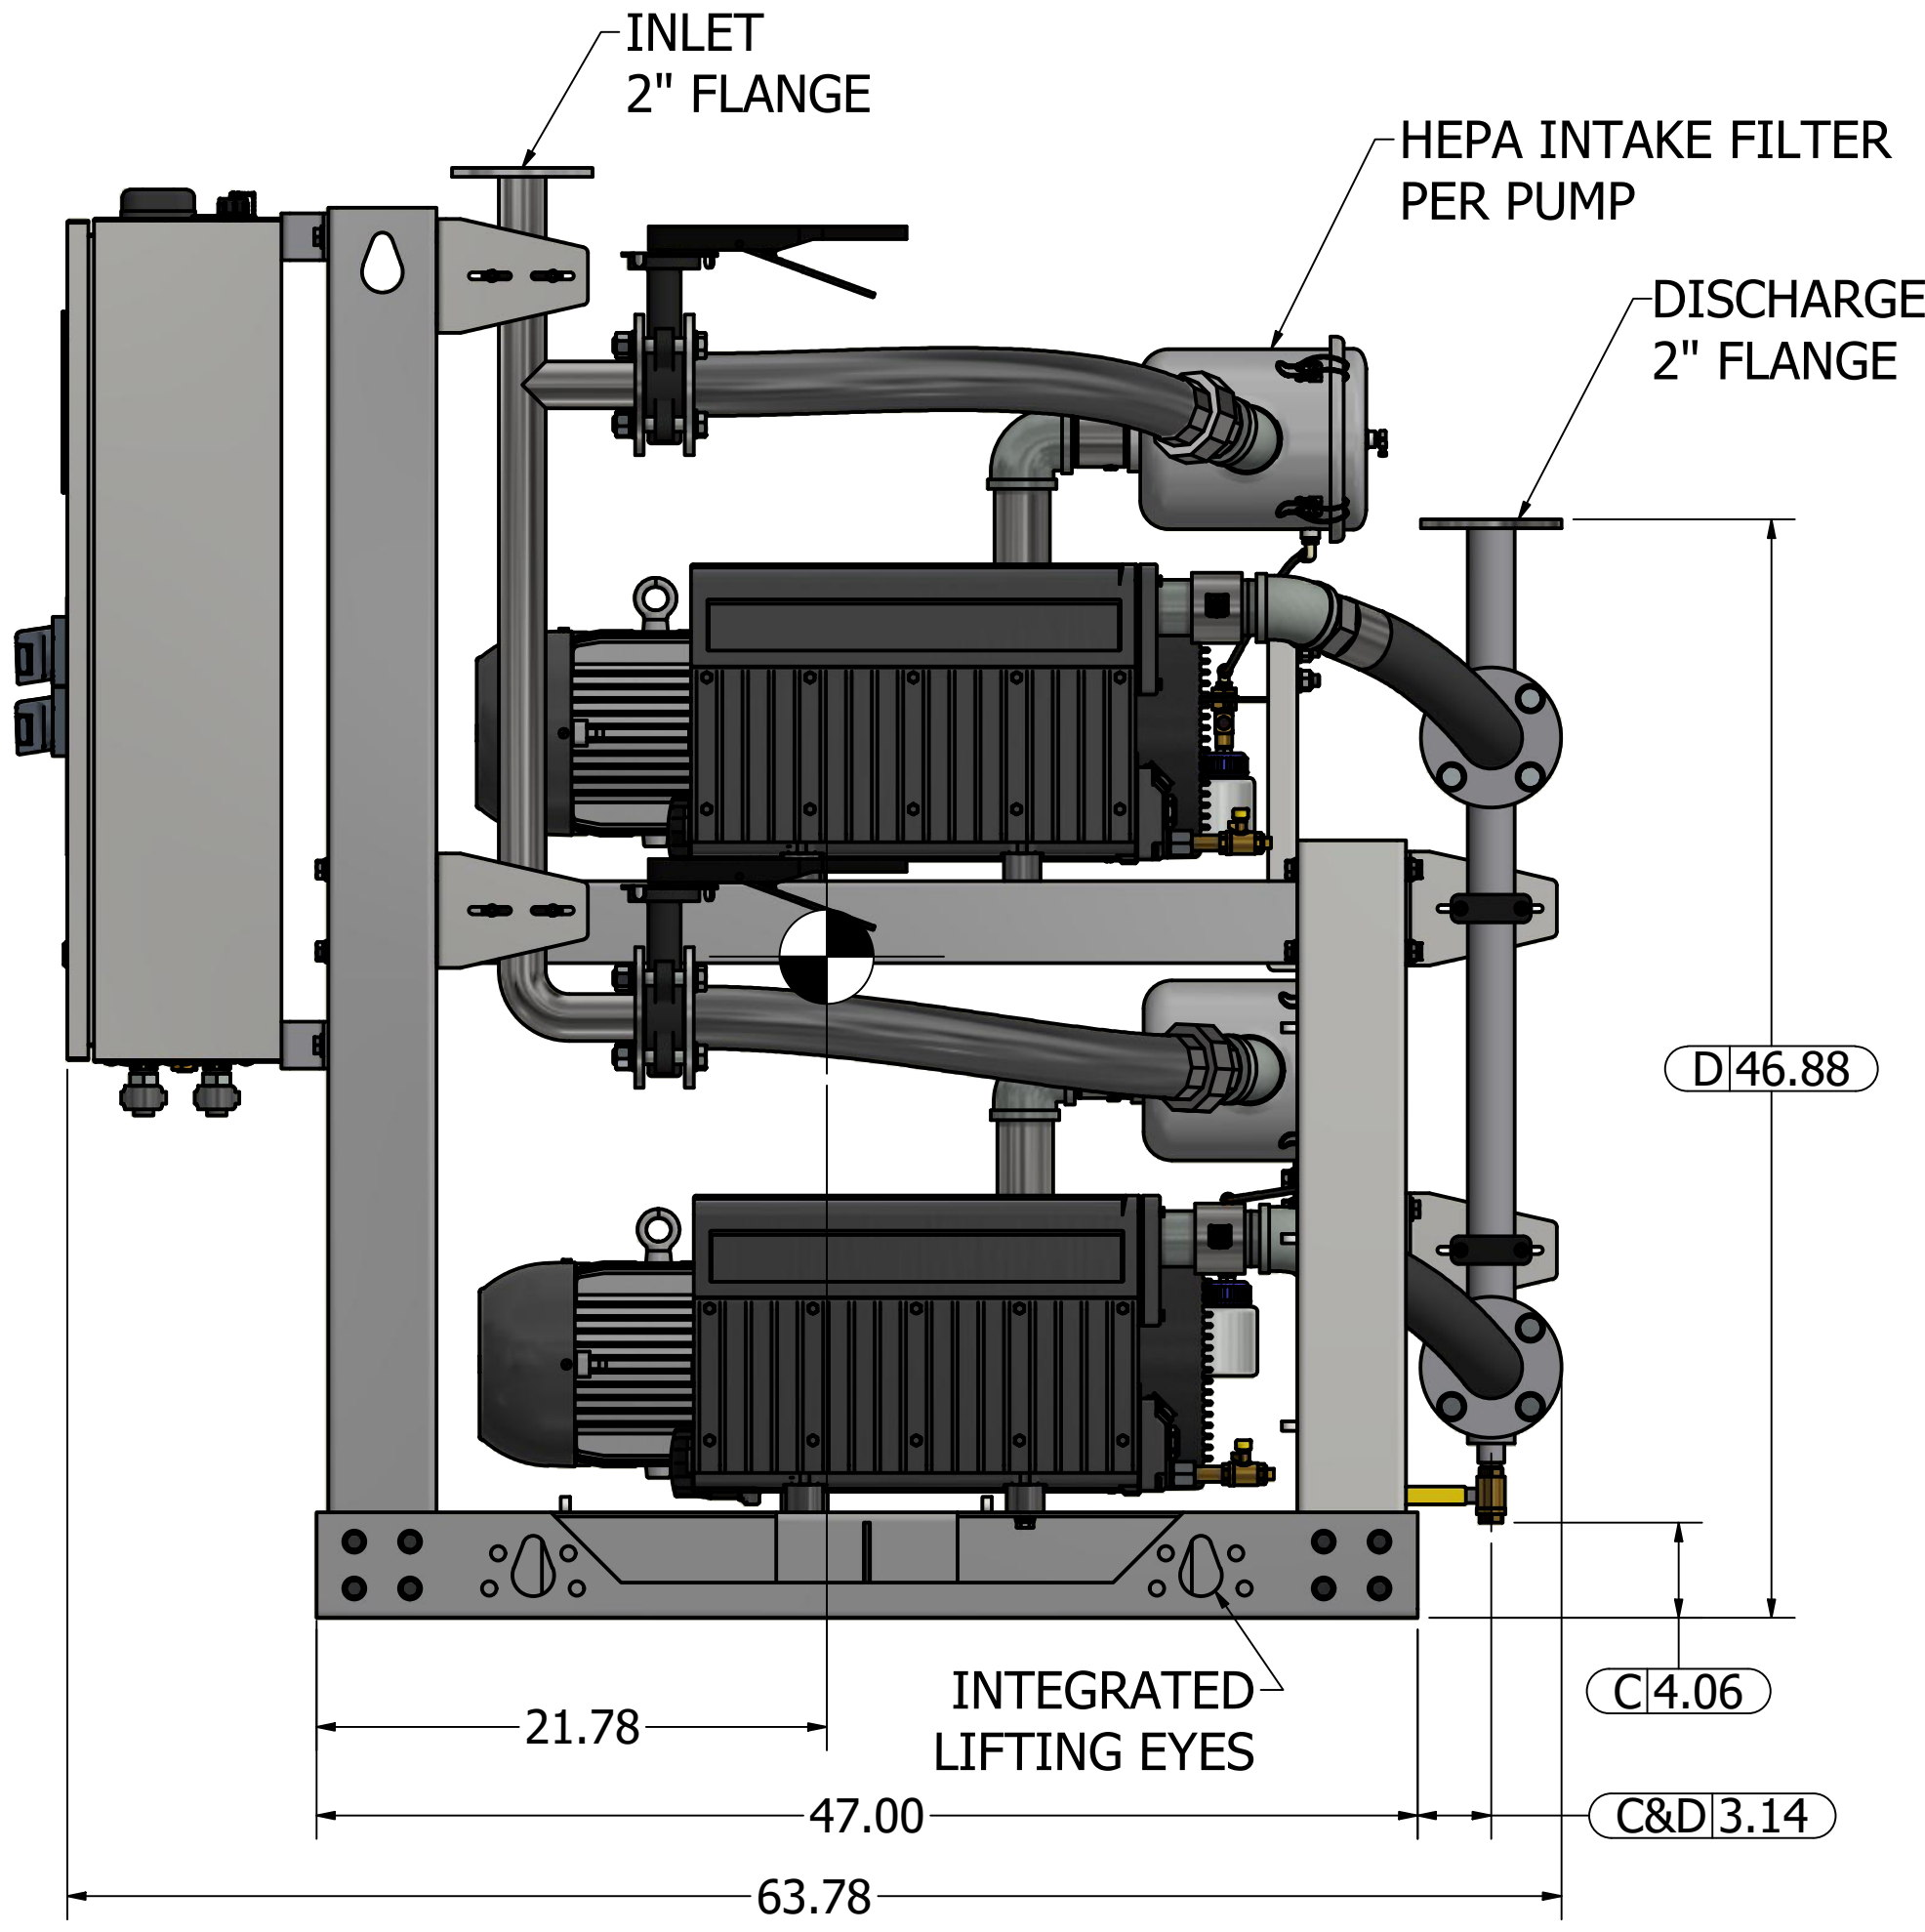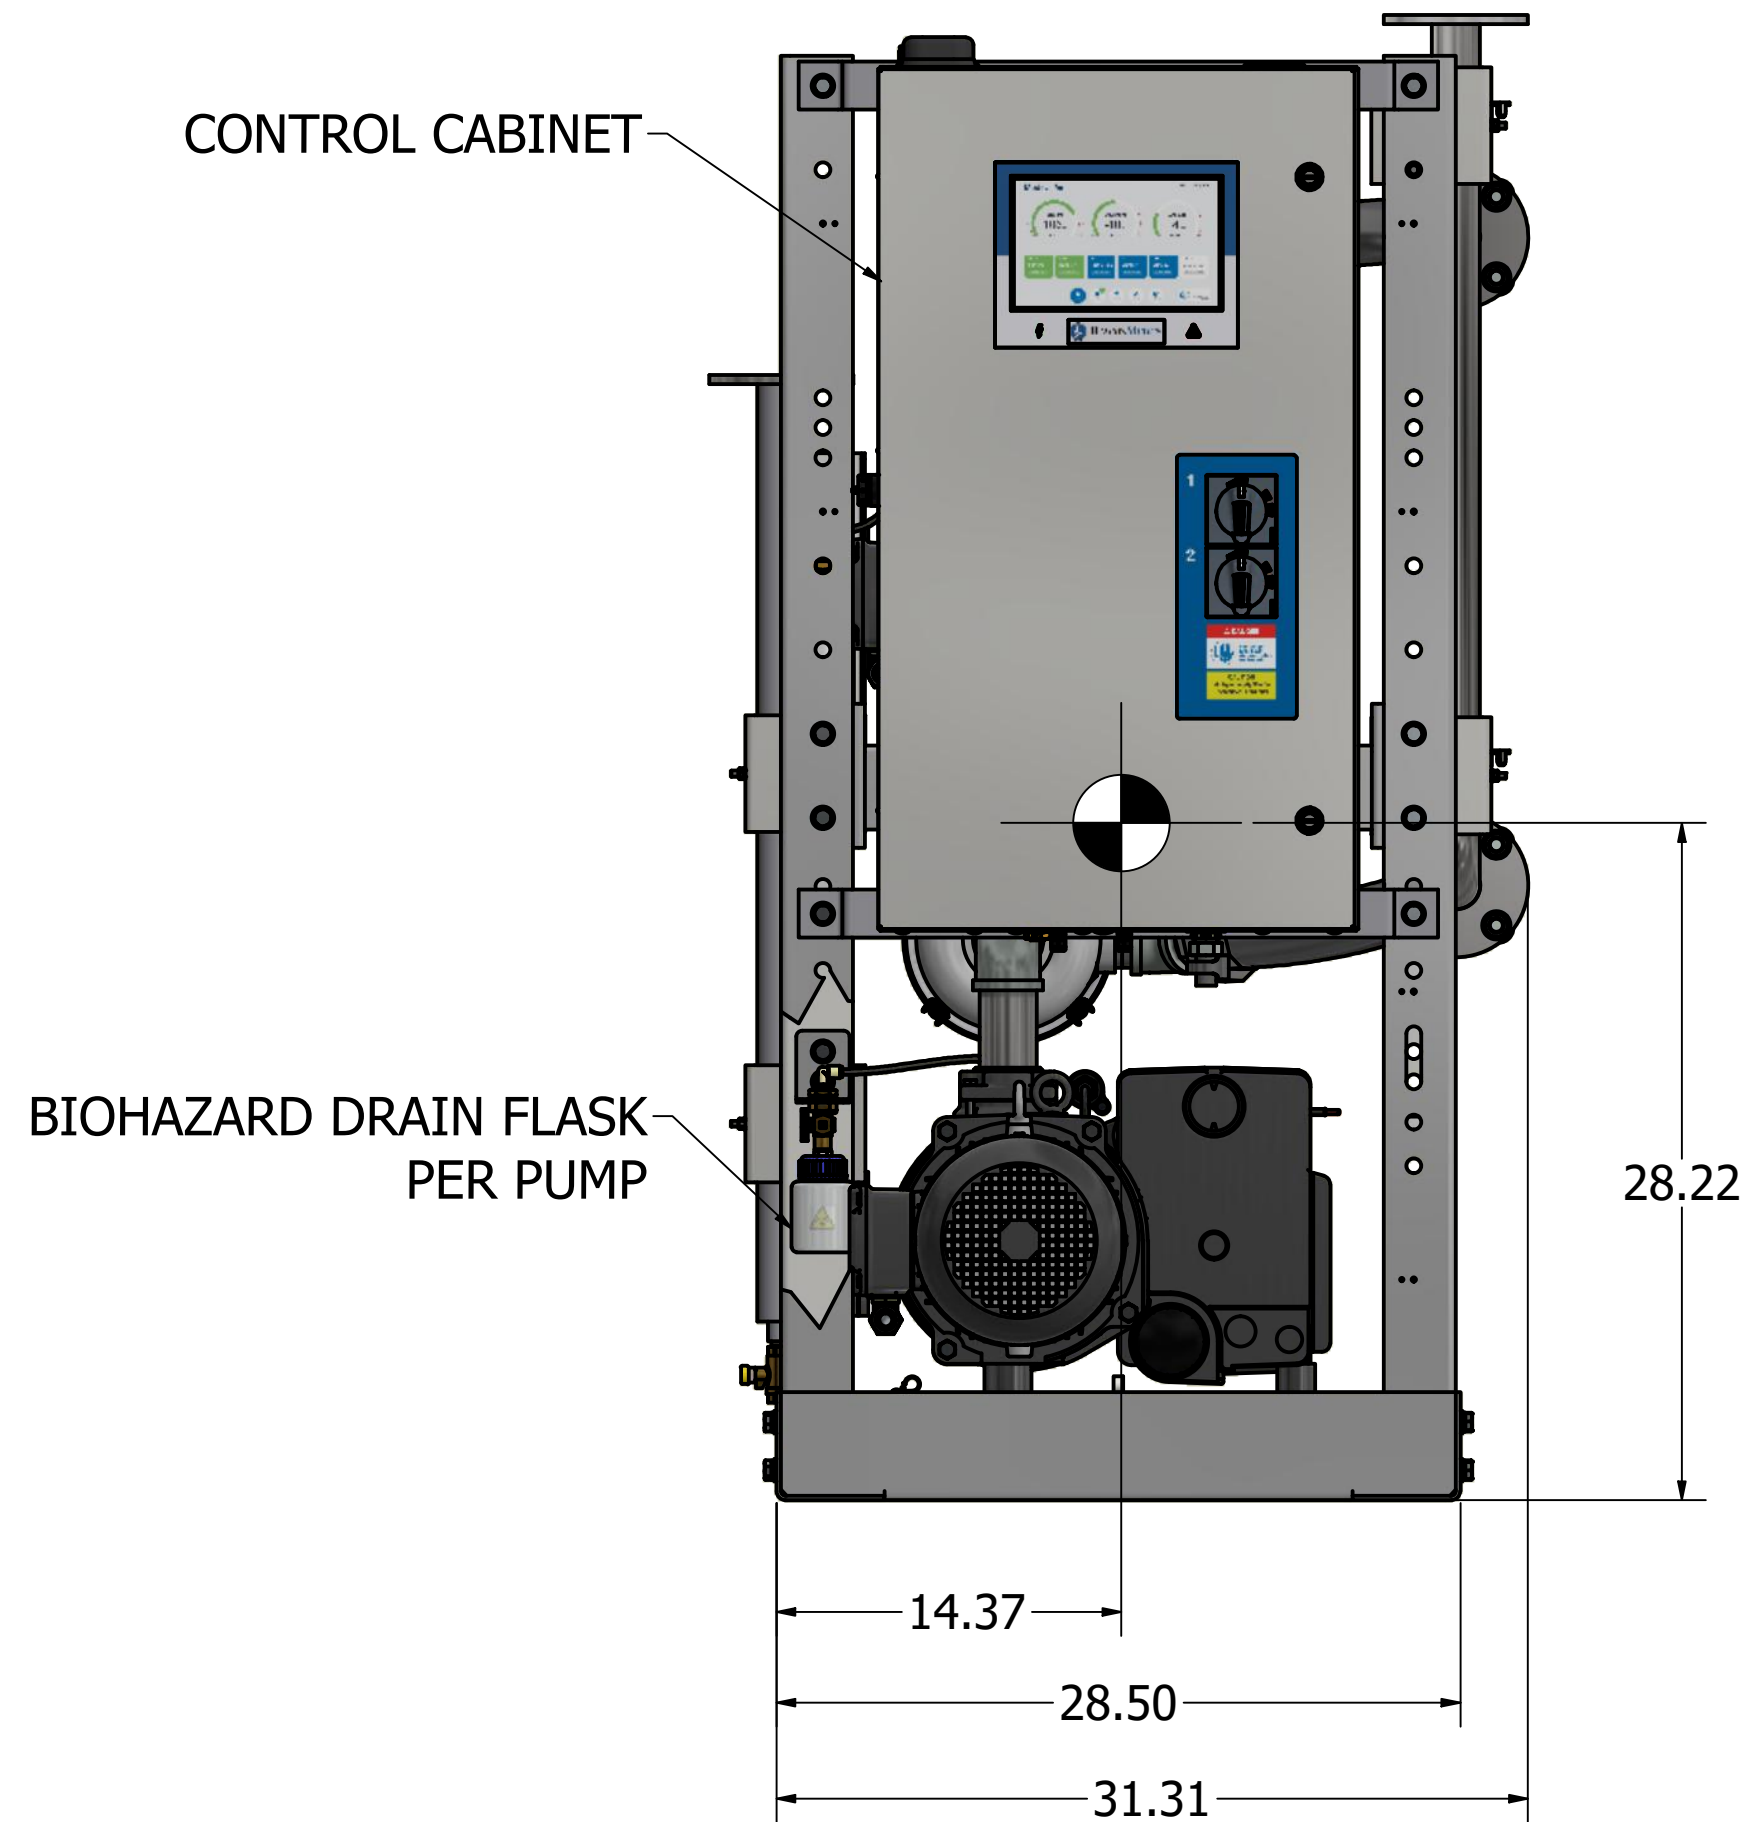

Revised: APS	Date: 3/24/2023	Drawn: USNkW	Date: 10/20/2010
	This drawing and the information contained therein remain the property of BeaconMedaes and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedaes Engineering.		
Description: GENERAL ASSEMBLY 5HP DX LUBE VAC MOD 240G RECEIVER	Part Number: 4107 8522 07	Rev: 04	Scale: D
Sheet 1 of 1	DO NOT SCALE THIS DOCUMENT		