This drawing and the Information contained thereon remain the property of BeaconMedæs and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedæs Engineering.

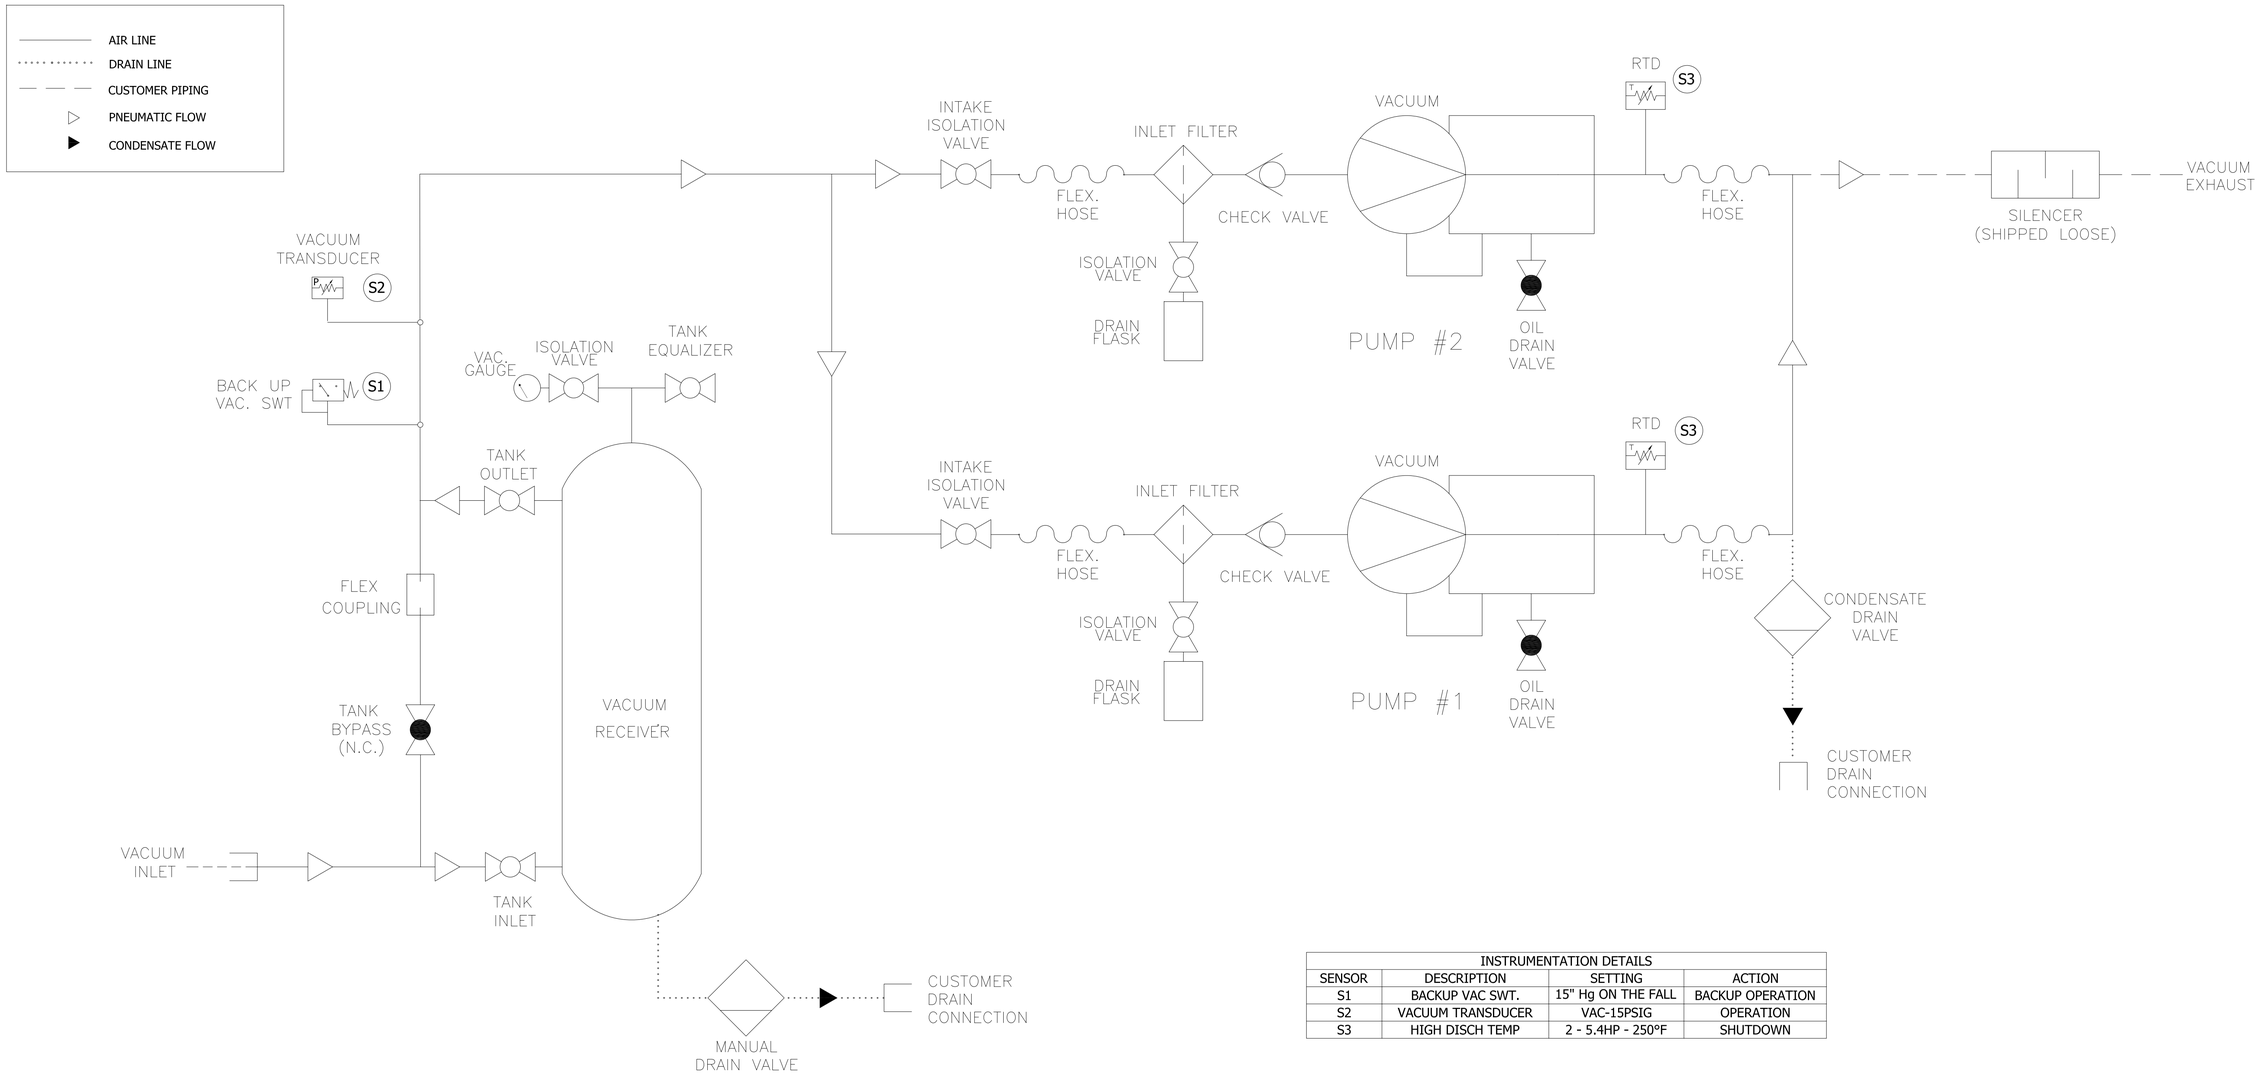

INSTRUMENTATION DETAILS			
SENSOR	DESCRIPTION	SETTING	ACTION
S1	BACKUP VAC SWT.	15" Hg ON THE FALL	BACKUP OPERATION
S2	VACUUM TRANSDUCER	VAC-15PSIG	OPERATION
S3	HIGH DISCH TEMP	2 - 5.4HP - 250°F	SHUTDOWN

Revised: SMB	Date: 12/10/20	Drawn: JDY	Date: 01/12/10
BeaconMedæs	UNLESS OTHERWISE SPECIFIED ALL DIMENSIONS ARE IN INCHES AND TOLERANCES ARE: .XX ± .02, .XXX ± .005, .XXXX ±.0005, ANGLES ± 5	Scale: NTS	D
Description: PNEUMATIC DIAGRAM 2-5.4HP DX CLAW VAC STACK MOUNT STANDARD & O2 ASSURED	Part Number: 4107 8518 09		
	DN: HOP200662	Rev: 01	
	Sheet 1 of 1	DO NOT SCALE THIS DOCUMENT	