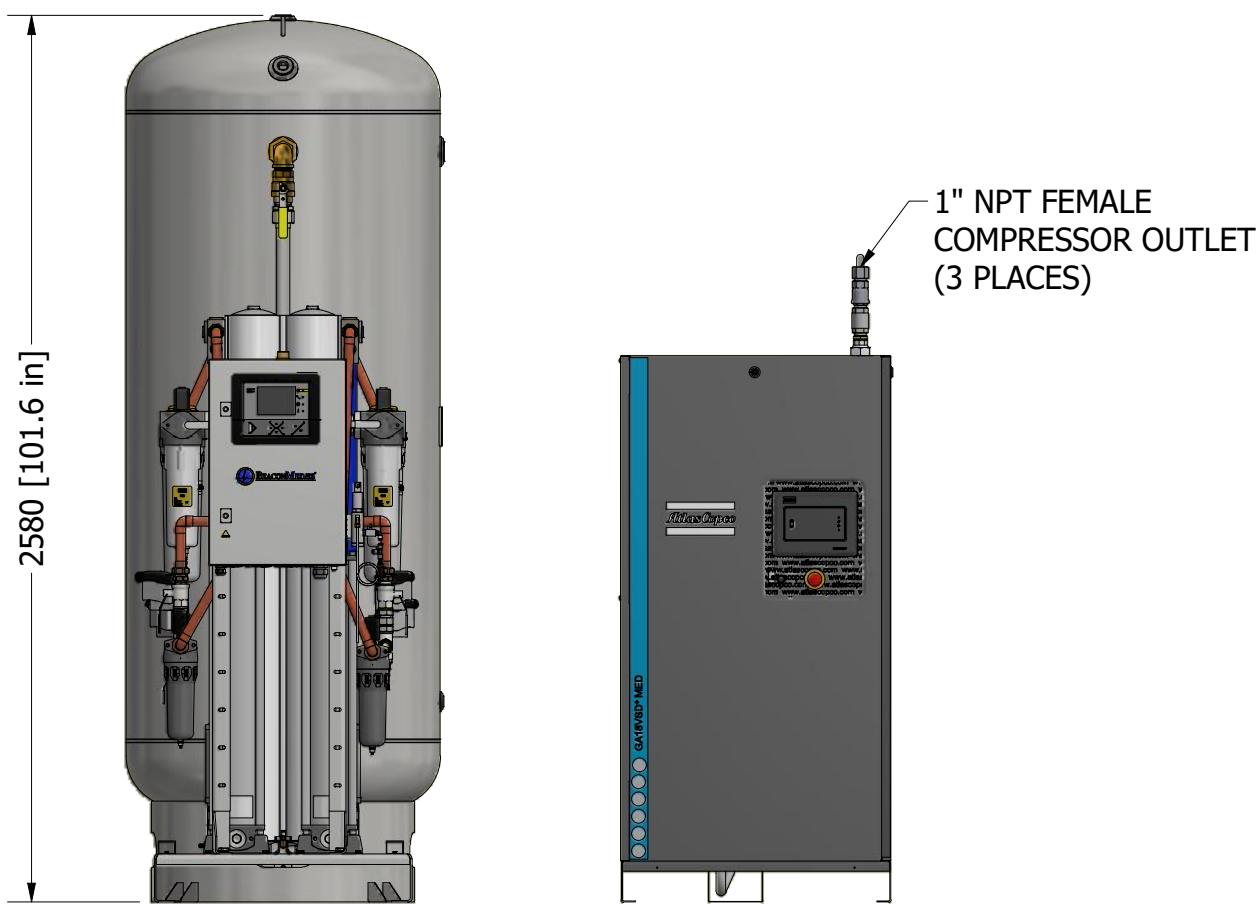


18. NO FOUNDATION OR INERTIA PAD IS REQUIRED. NO VIBRATION PADS ARE REQUIRED. HOUSEKEEPING PAD IS OPTIONAL.


Form F-007 Rev. 01

This drawing and the information contained thereon remain the property of BeaconMedaes and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedaes Engineering.



LINE KEY

SUPPLIED BY BEACONMEDAES	
24V AC
CAN COMMUNICATION CABLE

SUPPLIED BY OTHERS	
CONDENSATE DRAIN	- - - -
COPPER TUBE	_____

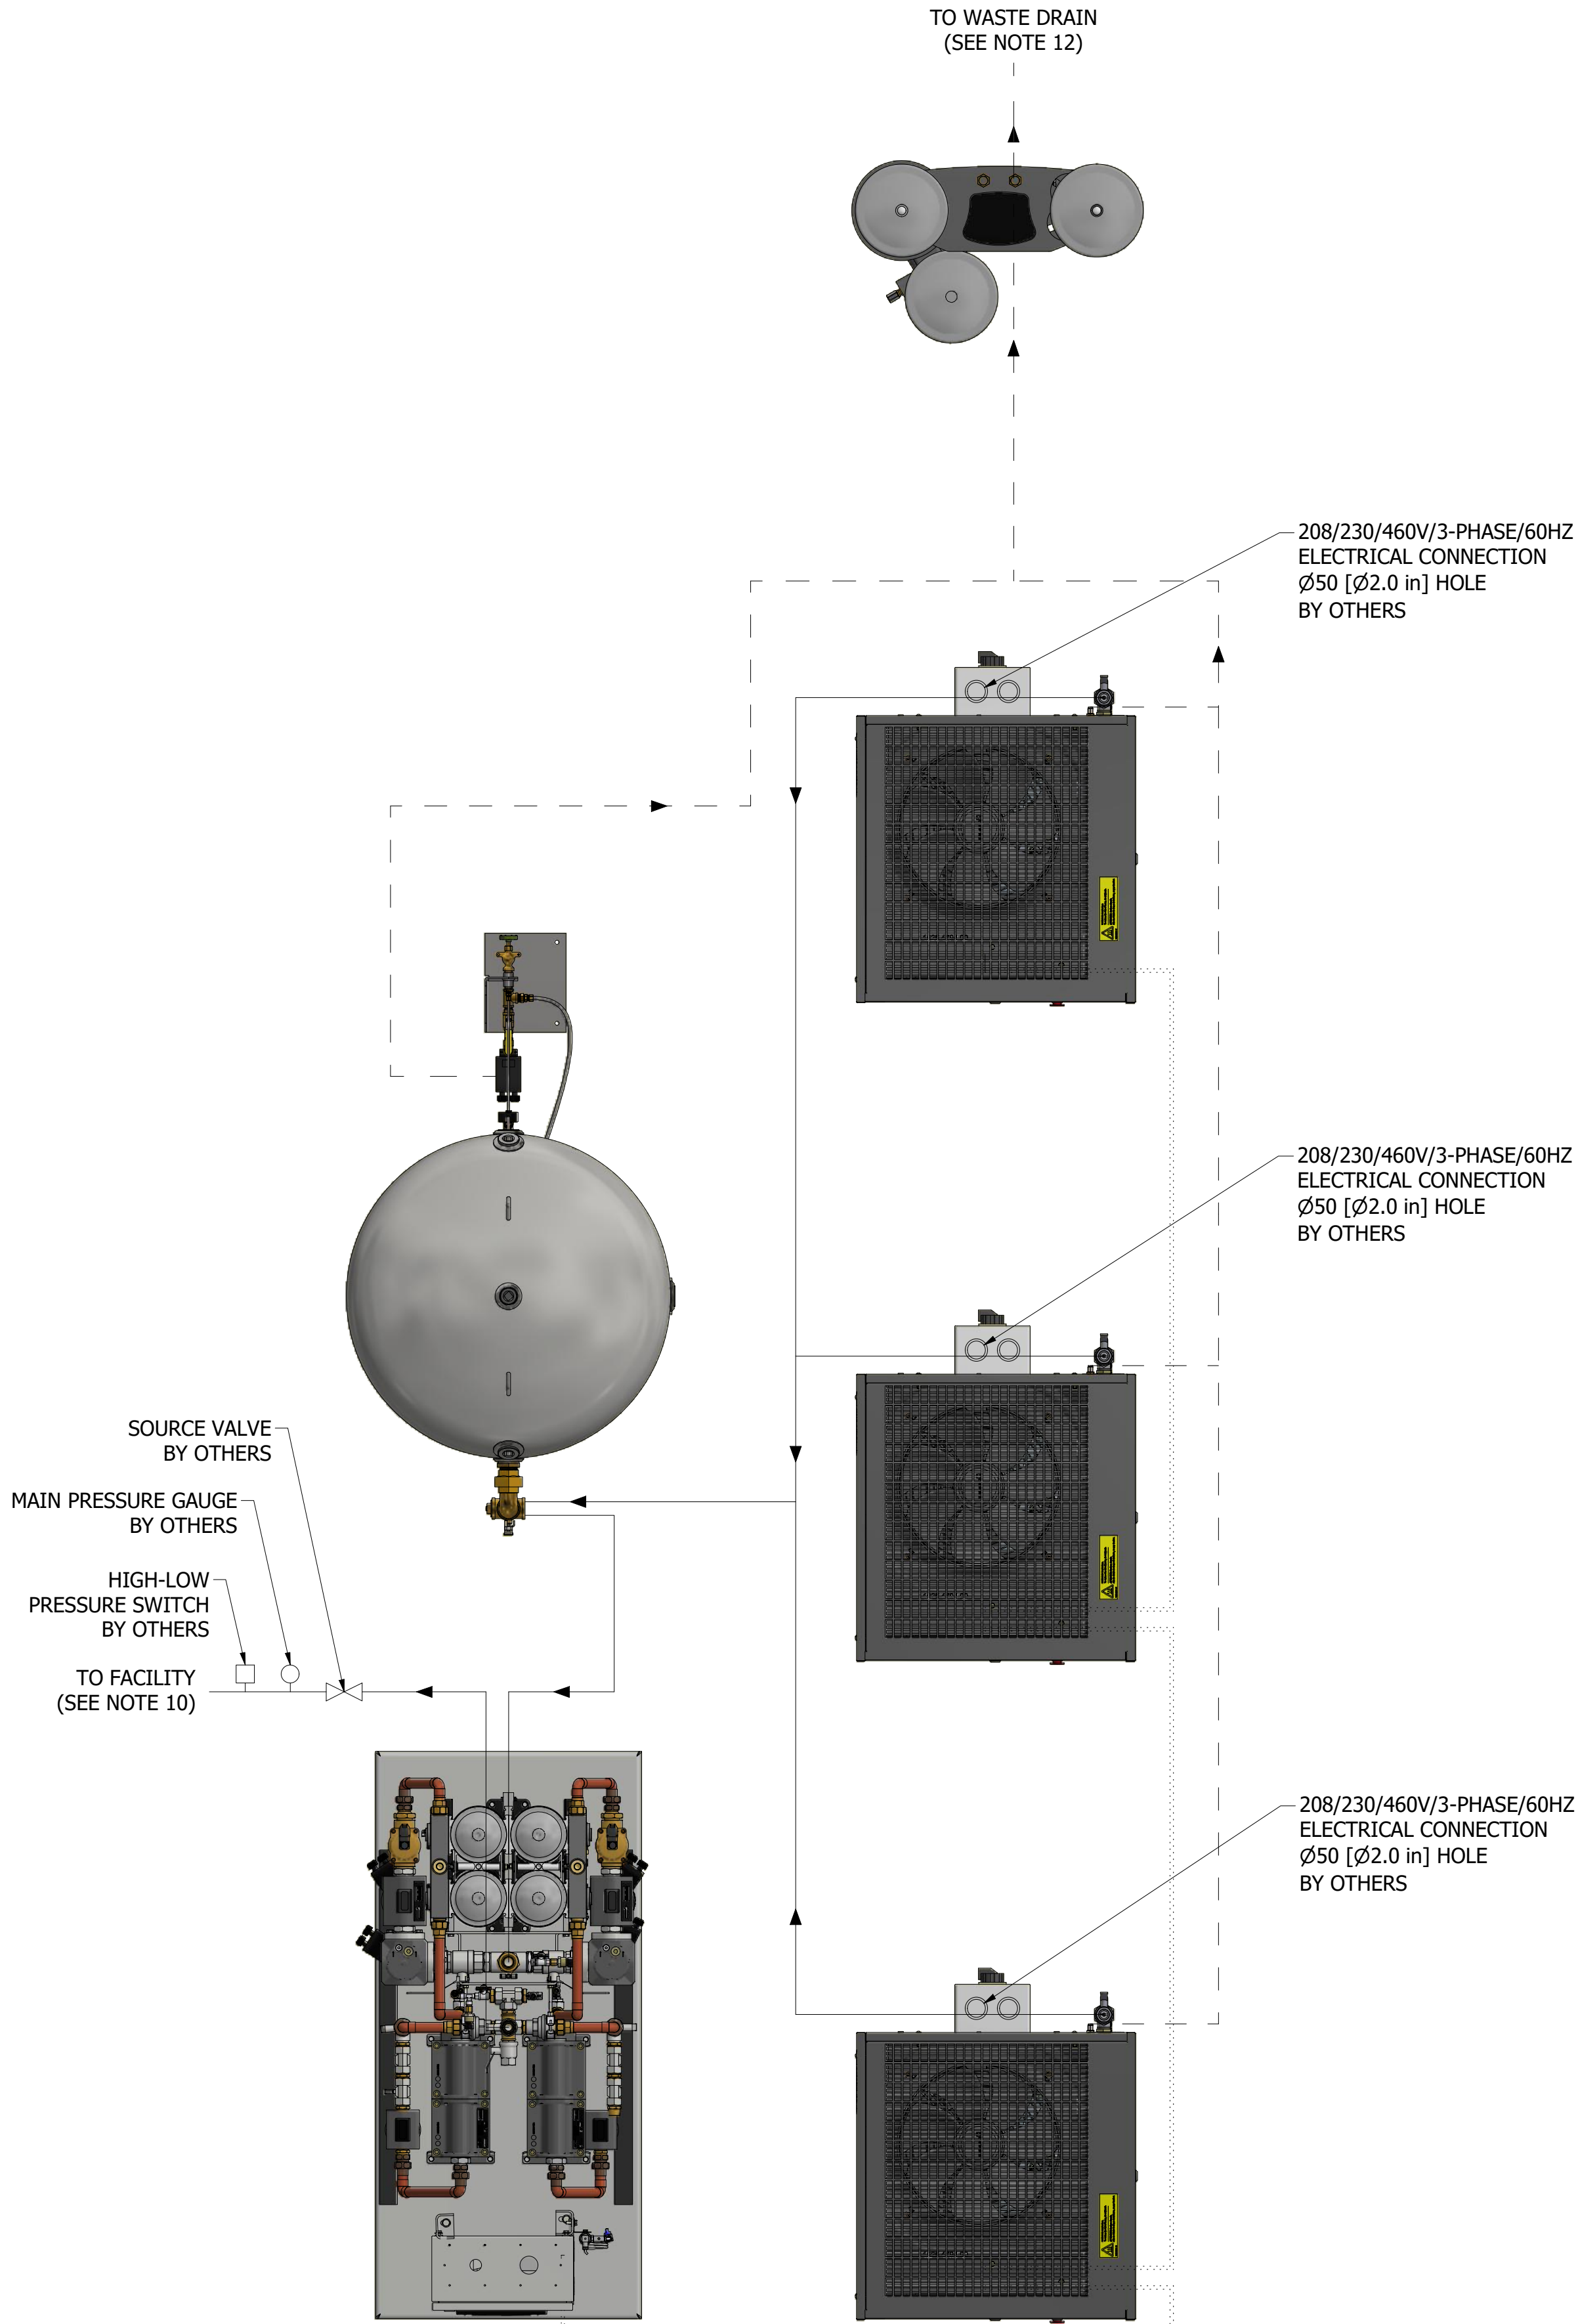

ANCHOR BOLT LOCATIONS

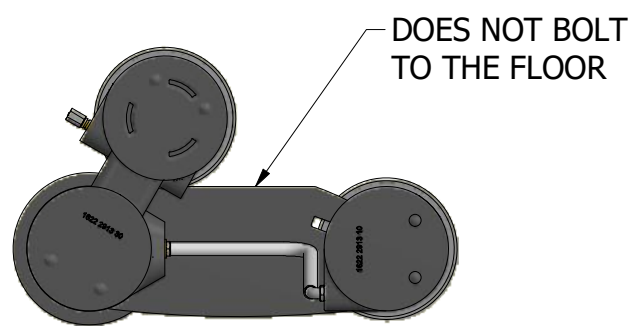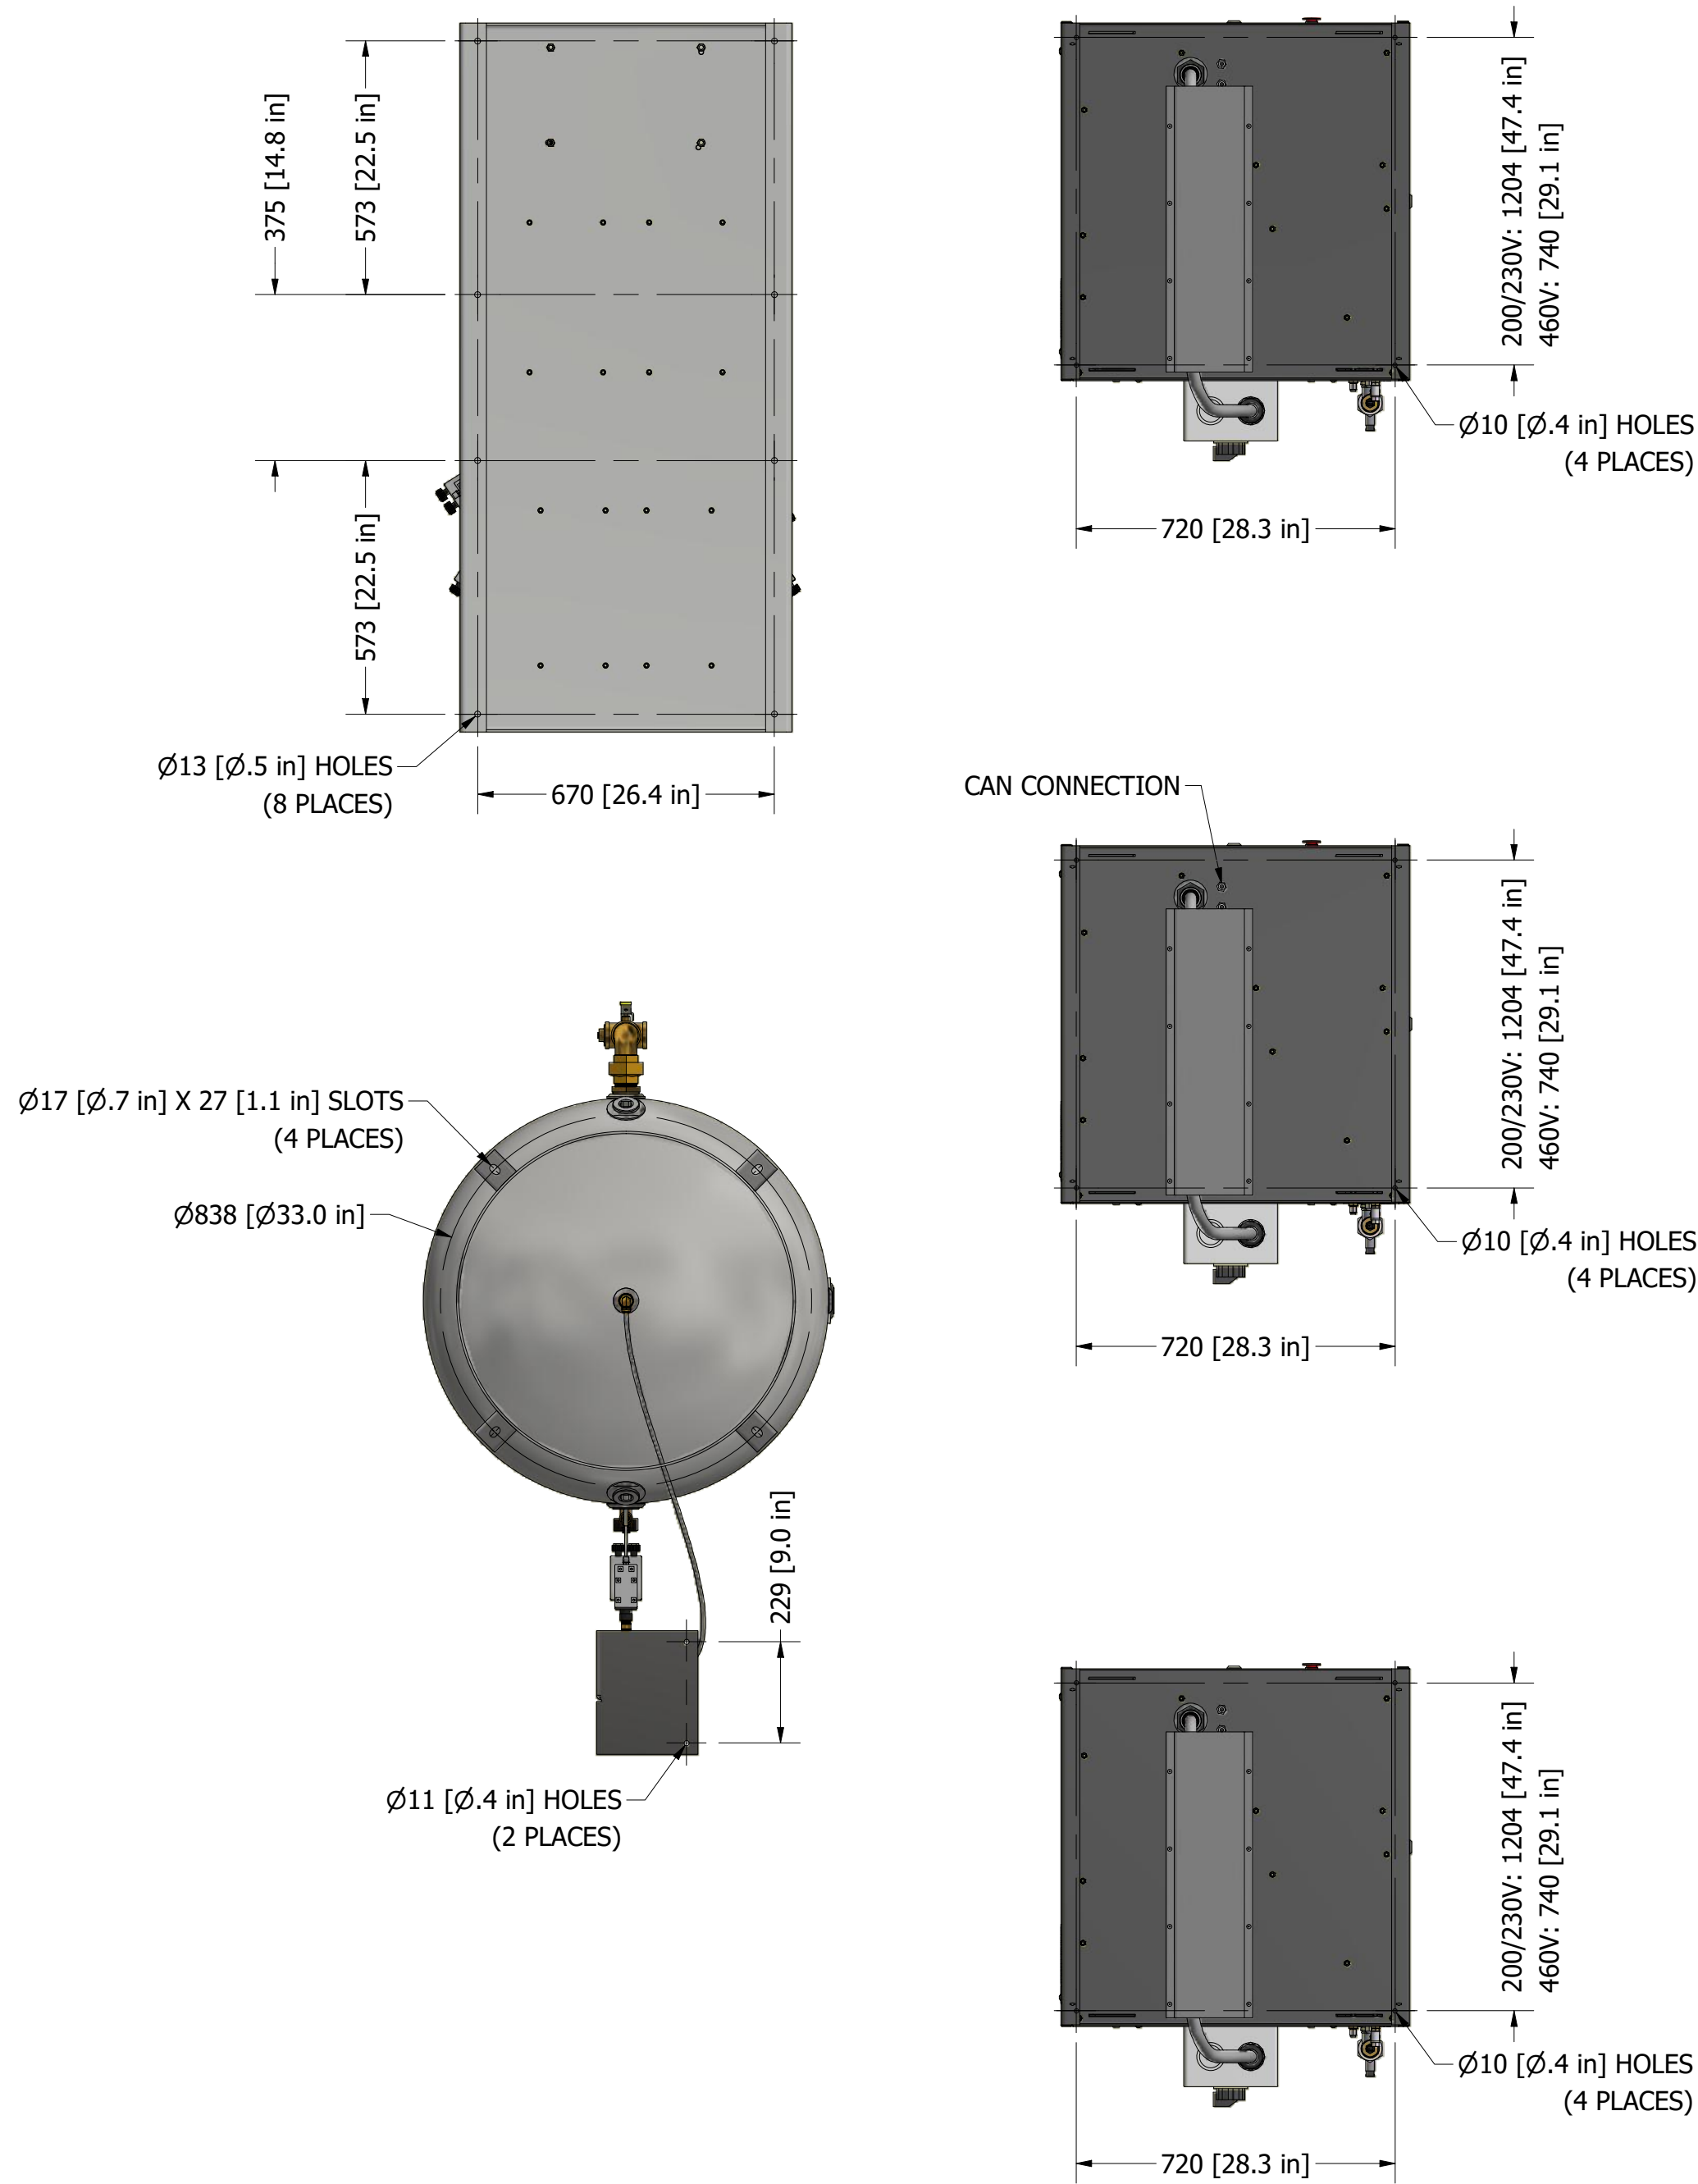

INSPECTION CHECKLIST UNLESS OTHERWISE SPECIFIED: ALL ITEMS MARKED BY ONE OF THE ABOVE SYMBOLS ARE TO BE INSPECTED EQUIPMENT TO BE USED DURING RECEIVING INSPECTION SHALL BE PER QUALITY SYSTEM PROCEDURES	Revised: GTM	Date: 3/25/2022	Drawn: SMB	Date: 12/16/2019
	UNLESS OTHERWISE SPECIFIED ALL DIMENSIONS ARE IN INCHES AND TOLERANCES ARE: XX ± .10 XXX ± .005		UNLESS OTHERWISE SPECIFIED ALL DIMENSIONS ARE IN INCHES AND TOLERANCES ARE: XXX ± .005 ANGLES ± .1	Scale: NTS
	Description: DWG INST TX 30HP INSTRUMENT AIR MODULAR		Drawing Number: 4107 8572 22	Rev: 02
	Sheet 2 of 2		DO NOT SCALE THIS DOCUMENT	