










Notes:

1. DISCHARGE MUFFLER WILL BE SHIPPED LOOSE.
2. DX MODULE W/PANEL WEIGHT: 1,874 LBS.
DX MODULE WEIGHT: 1,667 LBS. (INCLUDES
FUTURE EXPANSION PUMP)
240G TANK WEIGHT: 713 LBS
3.  INDICATES LIFTING POINT.
4.  DENOTES CENTER OF GRAVITY.
(INCLUDES FUTURE EXPANSION MODULE)

SYSTEM CONNECTIONS	
ID	DESCRIPTION
I	INLET LOCATION
D	DISCHARGE LOCATION
C	CONDENSATE DRAIN LOCATION
T	TANK DRAIN

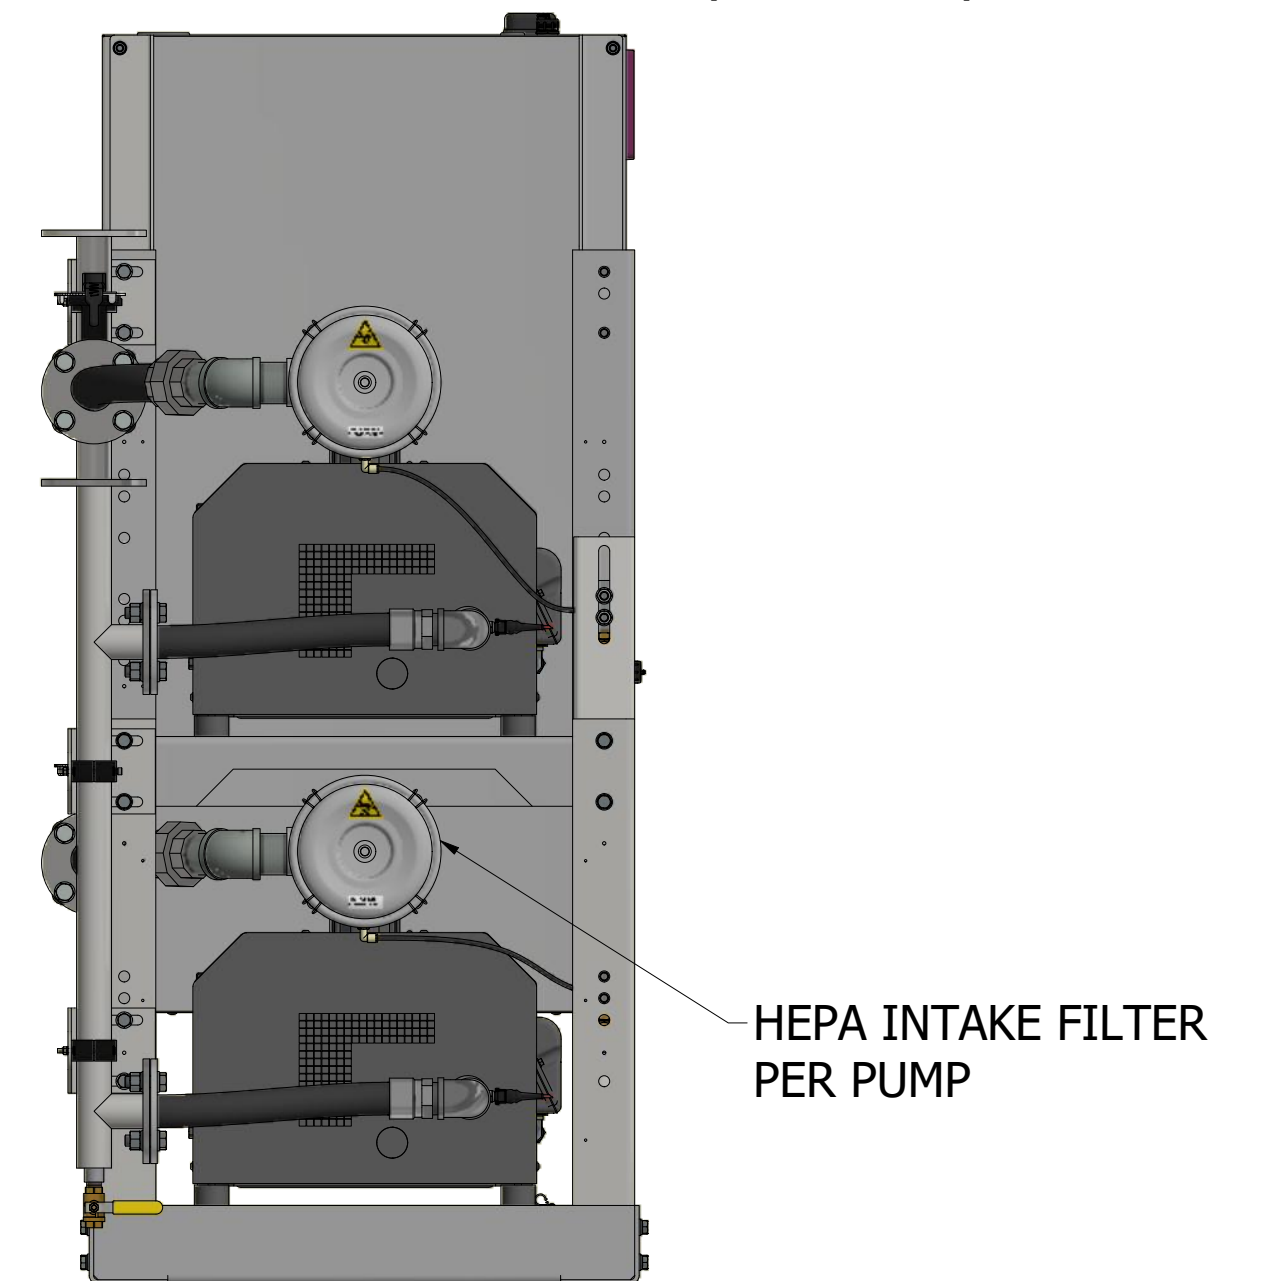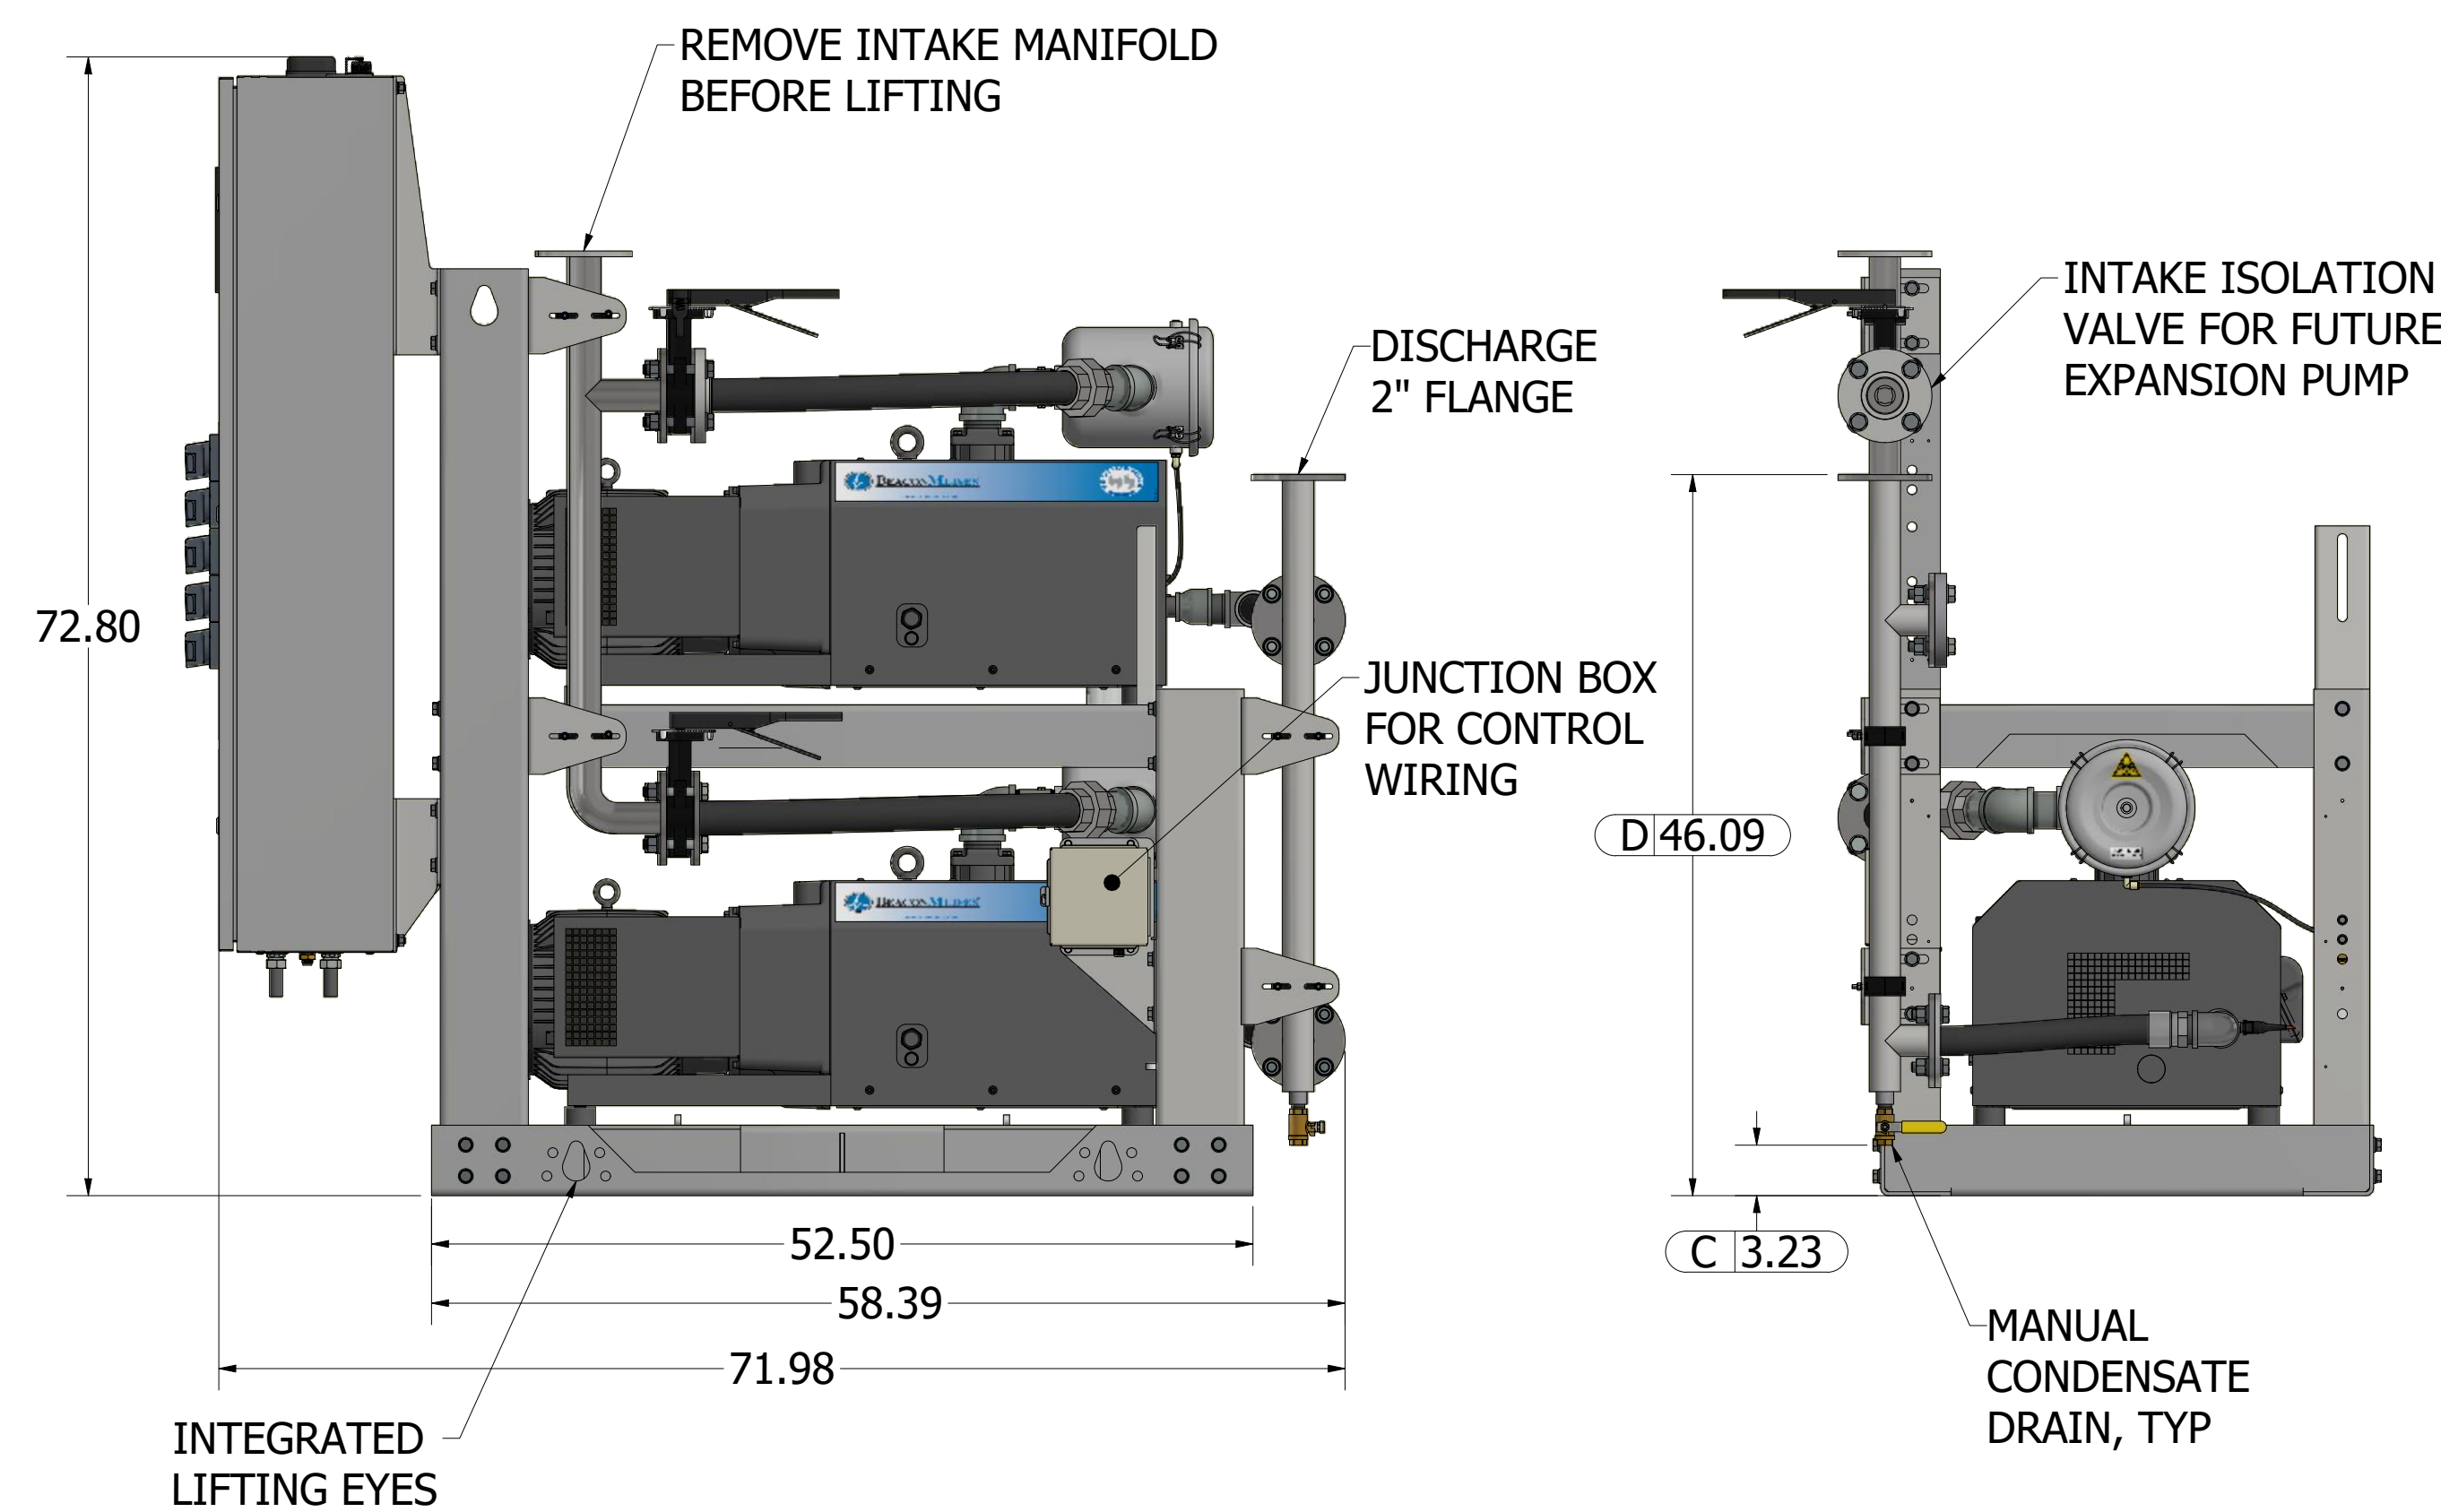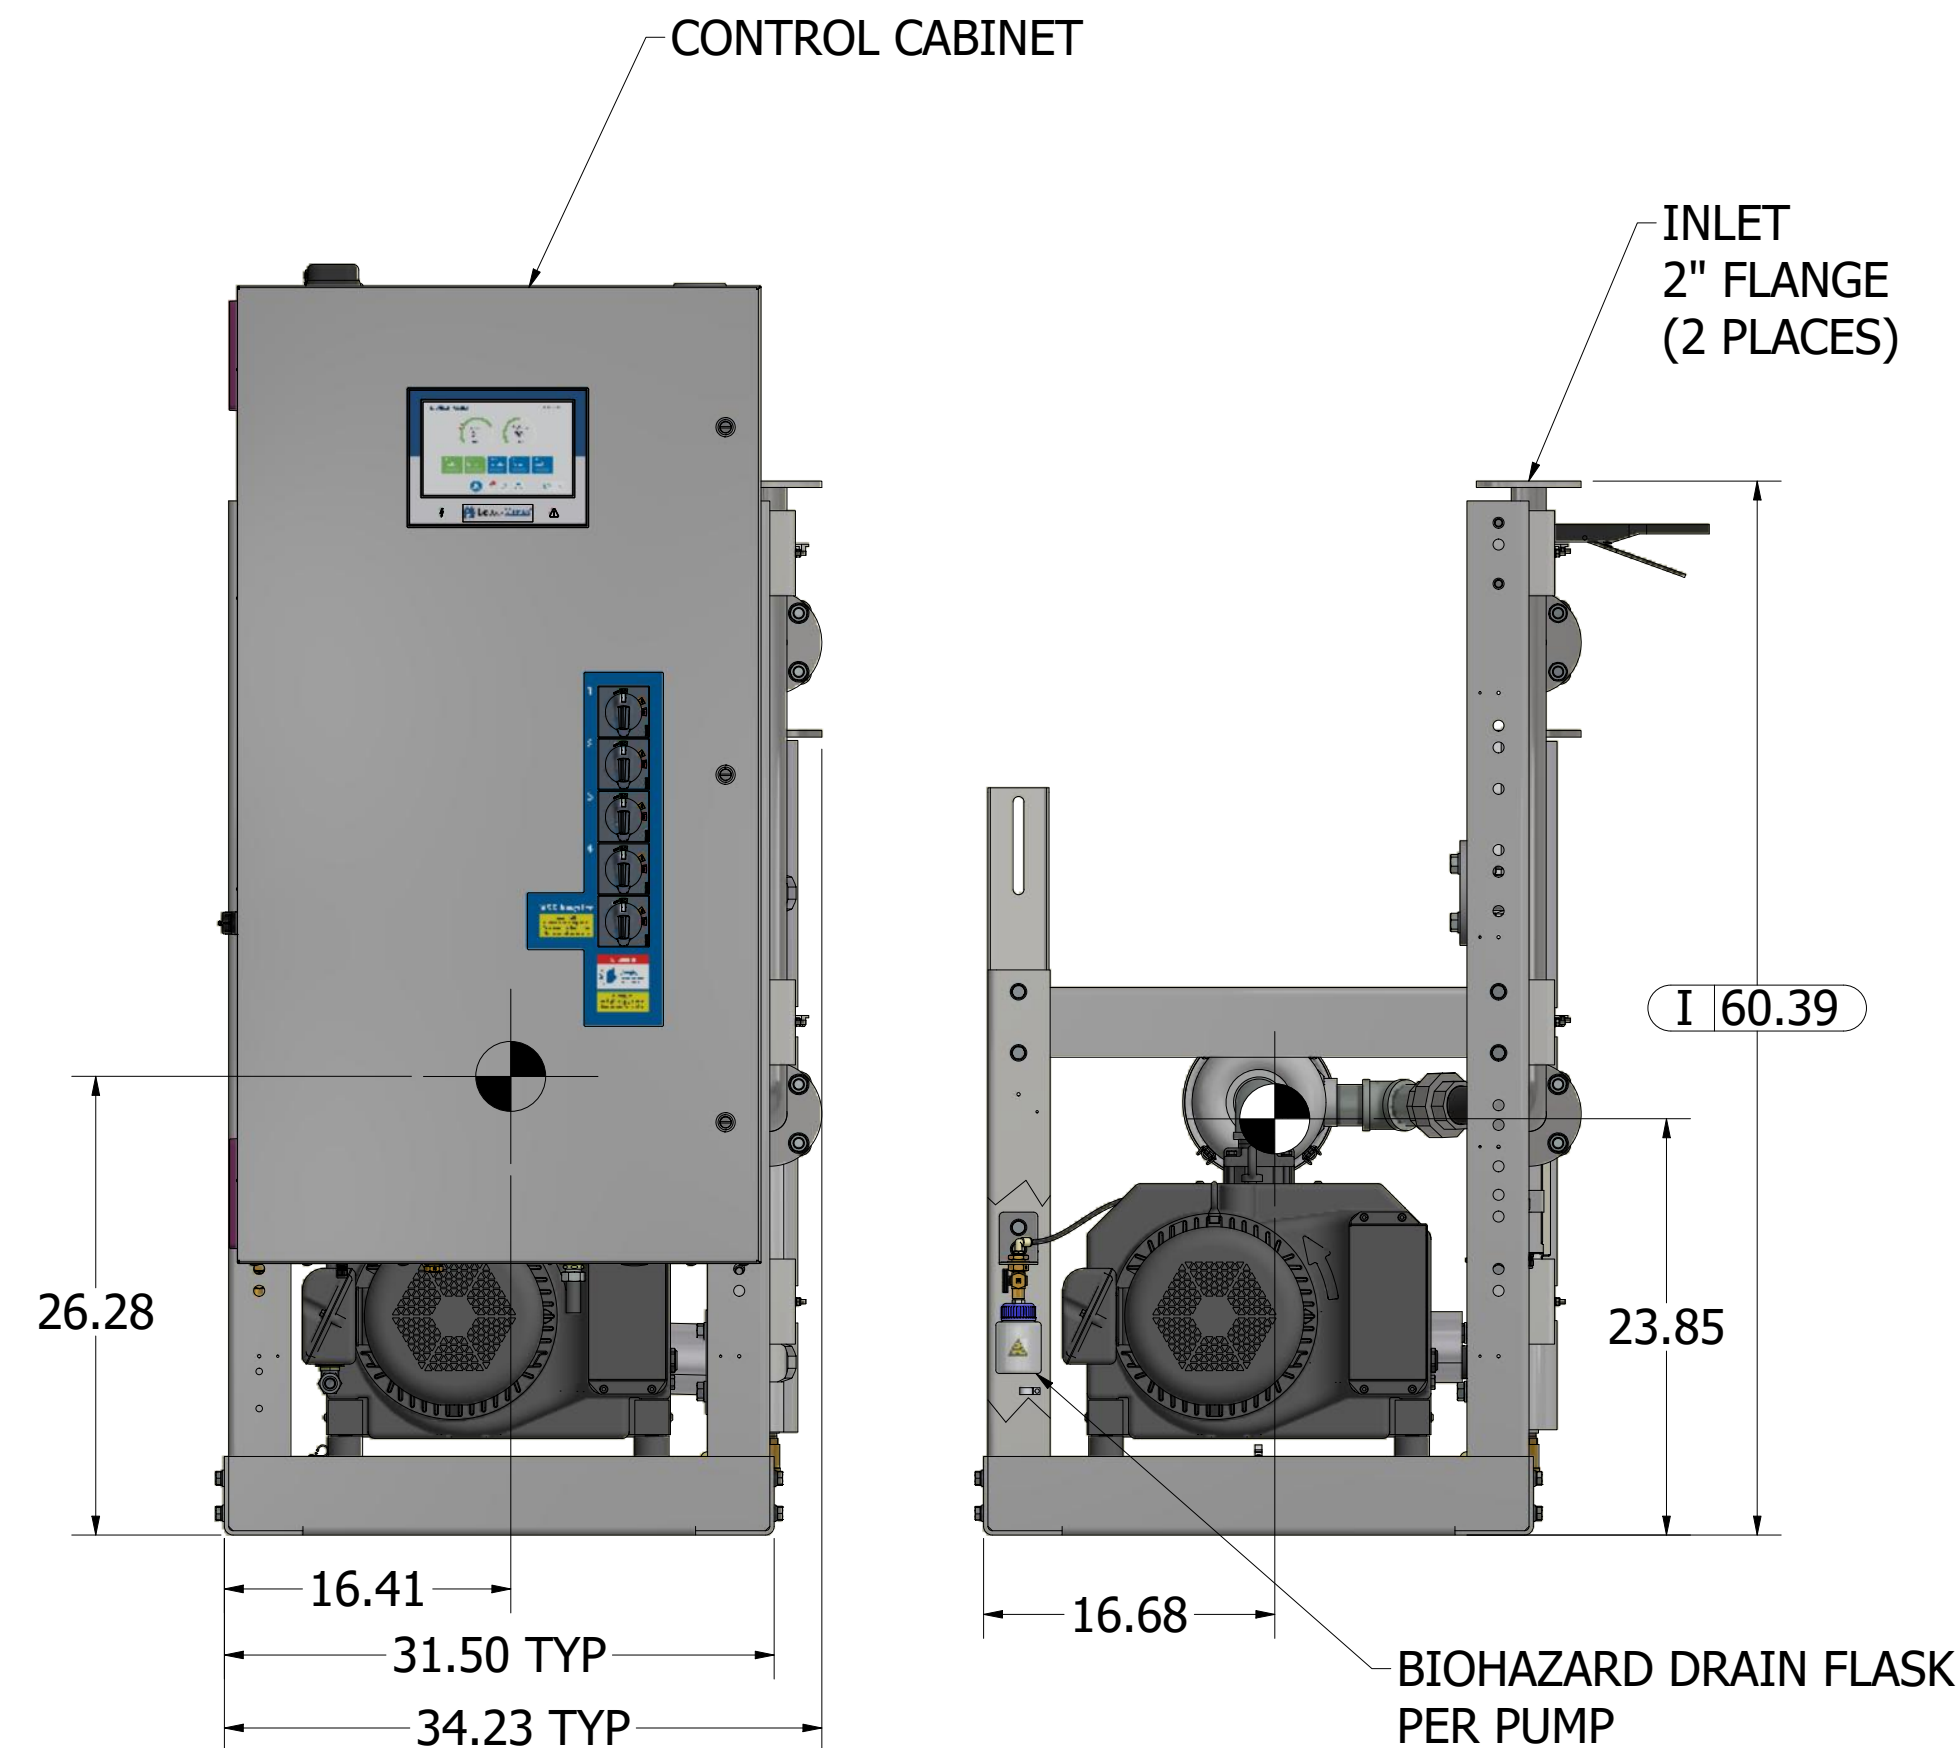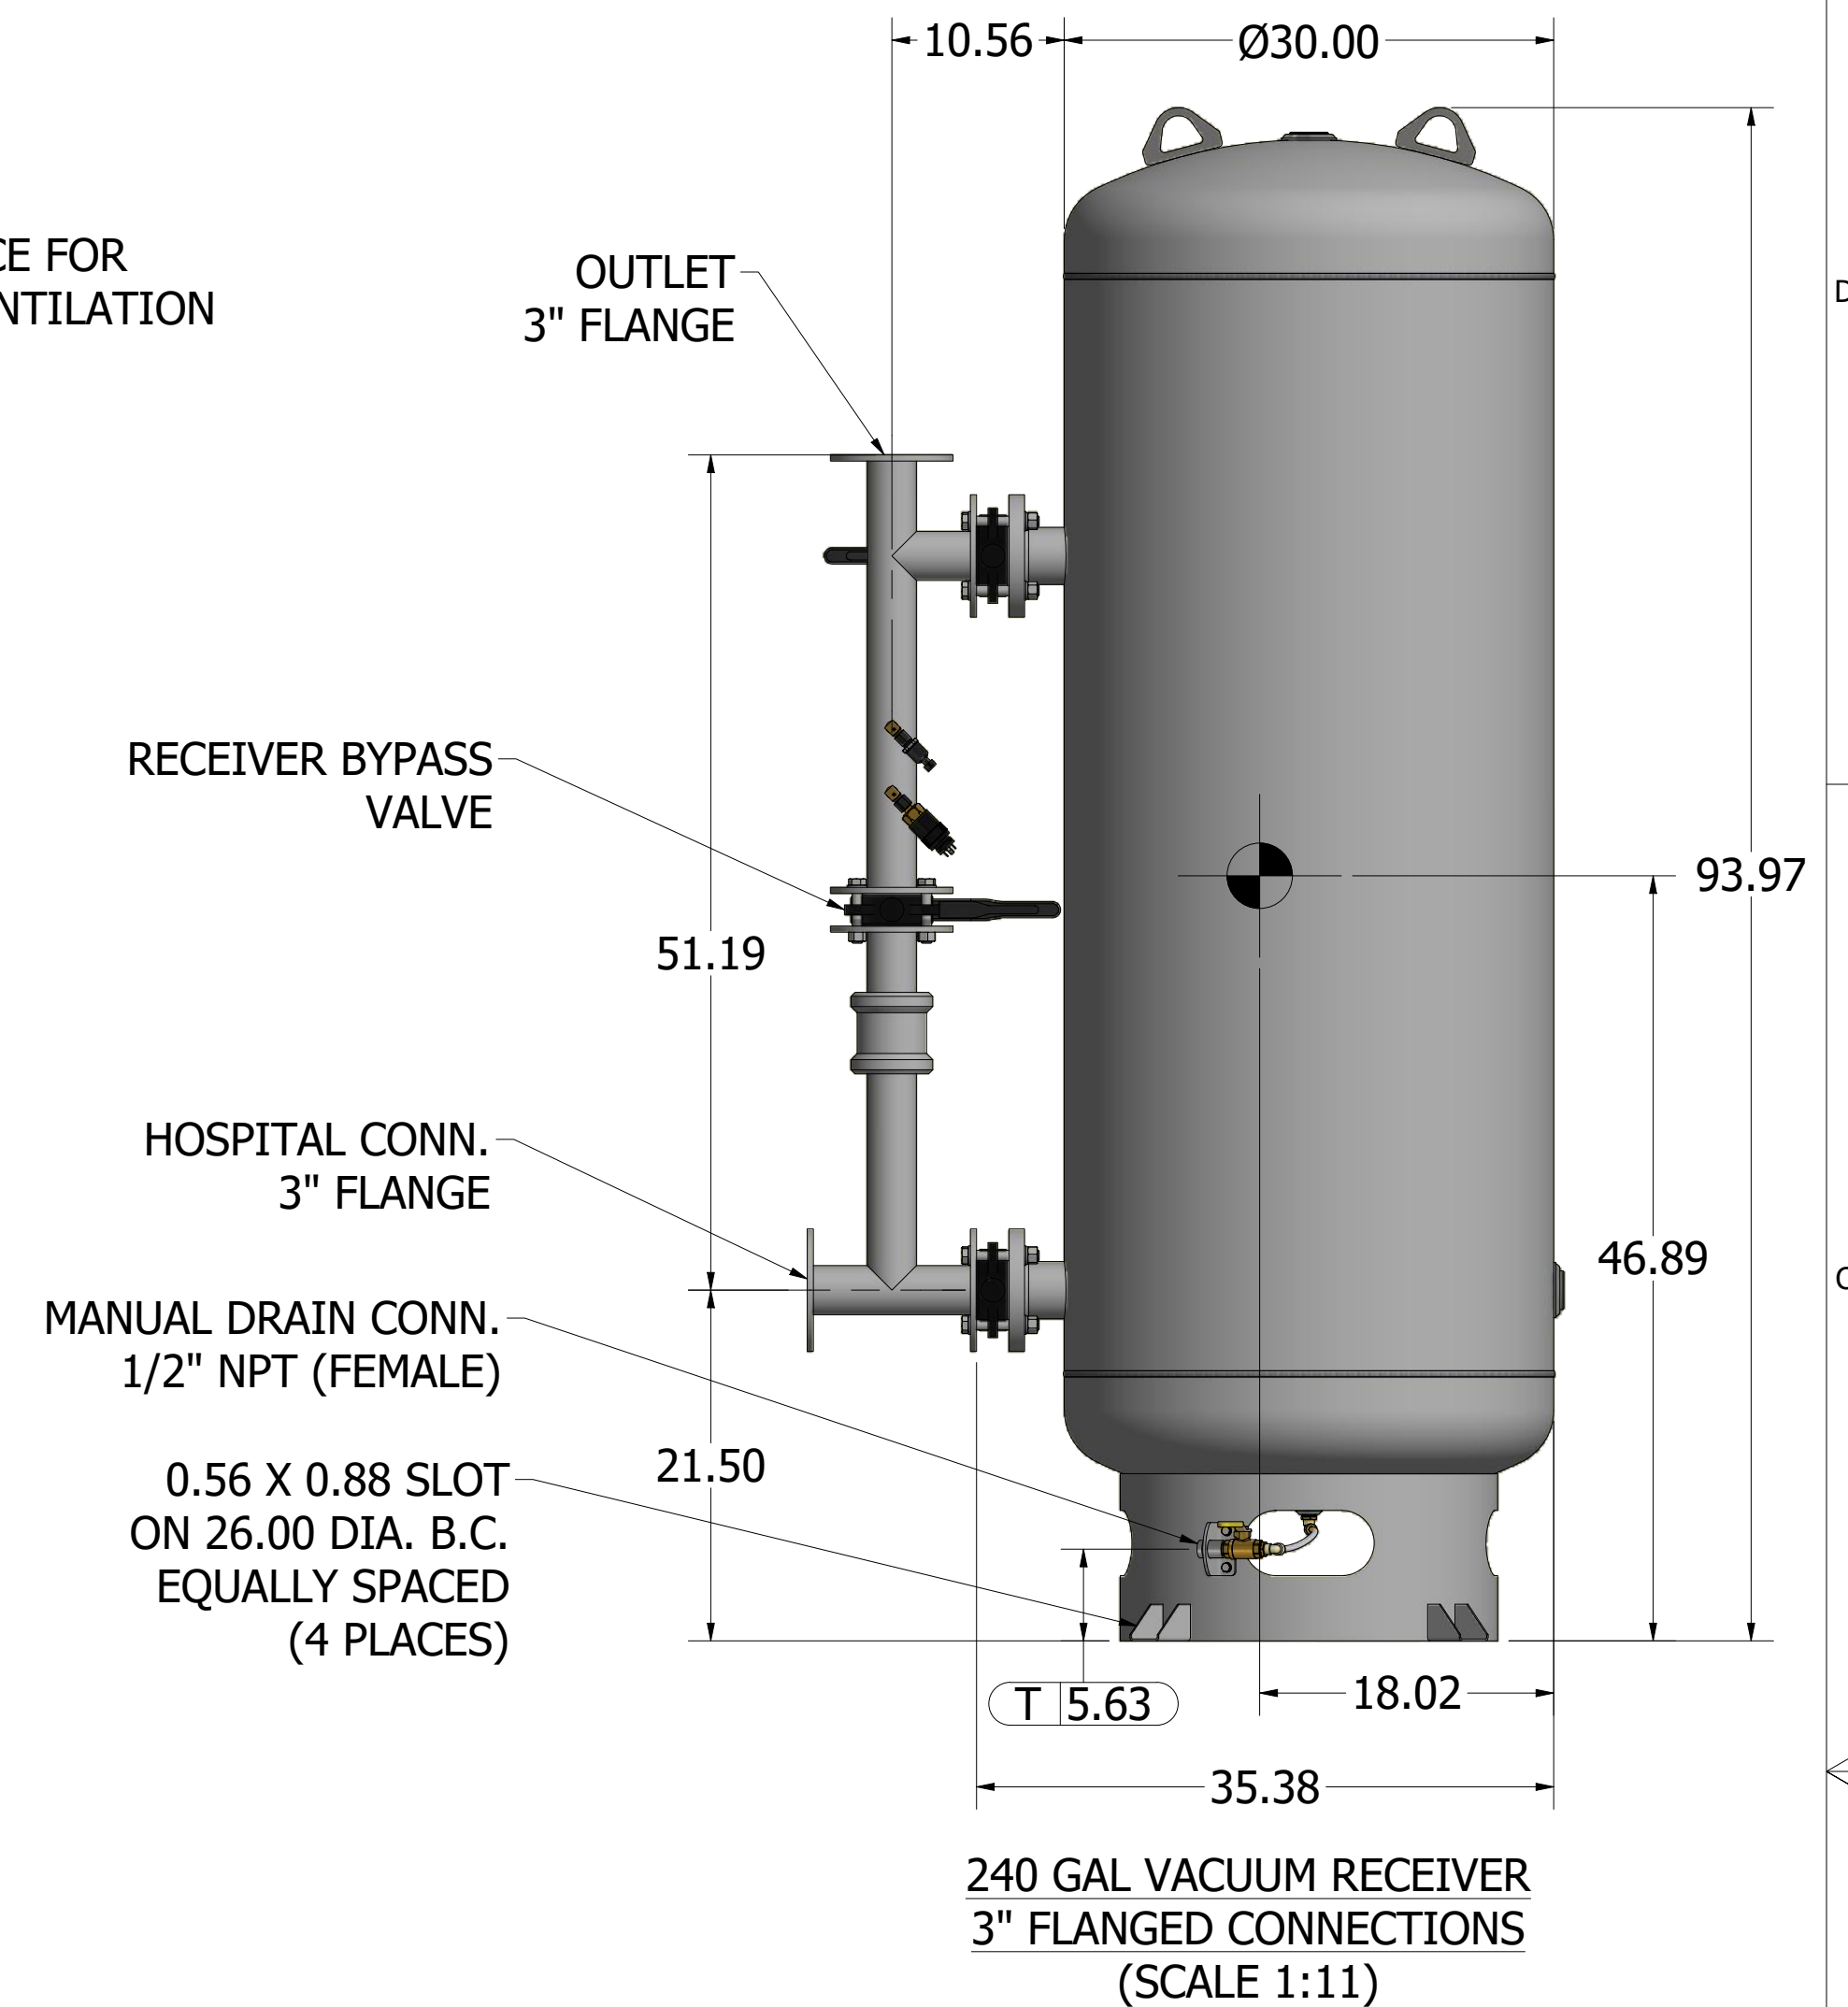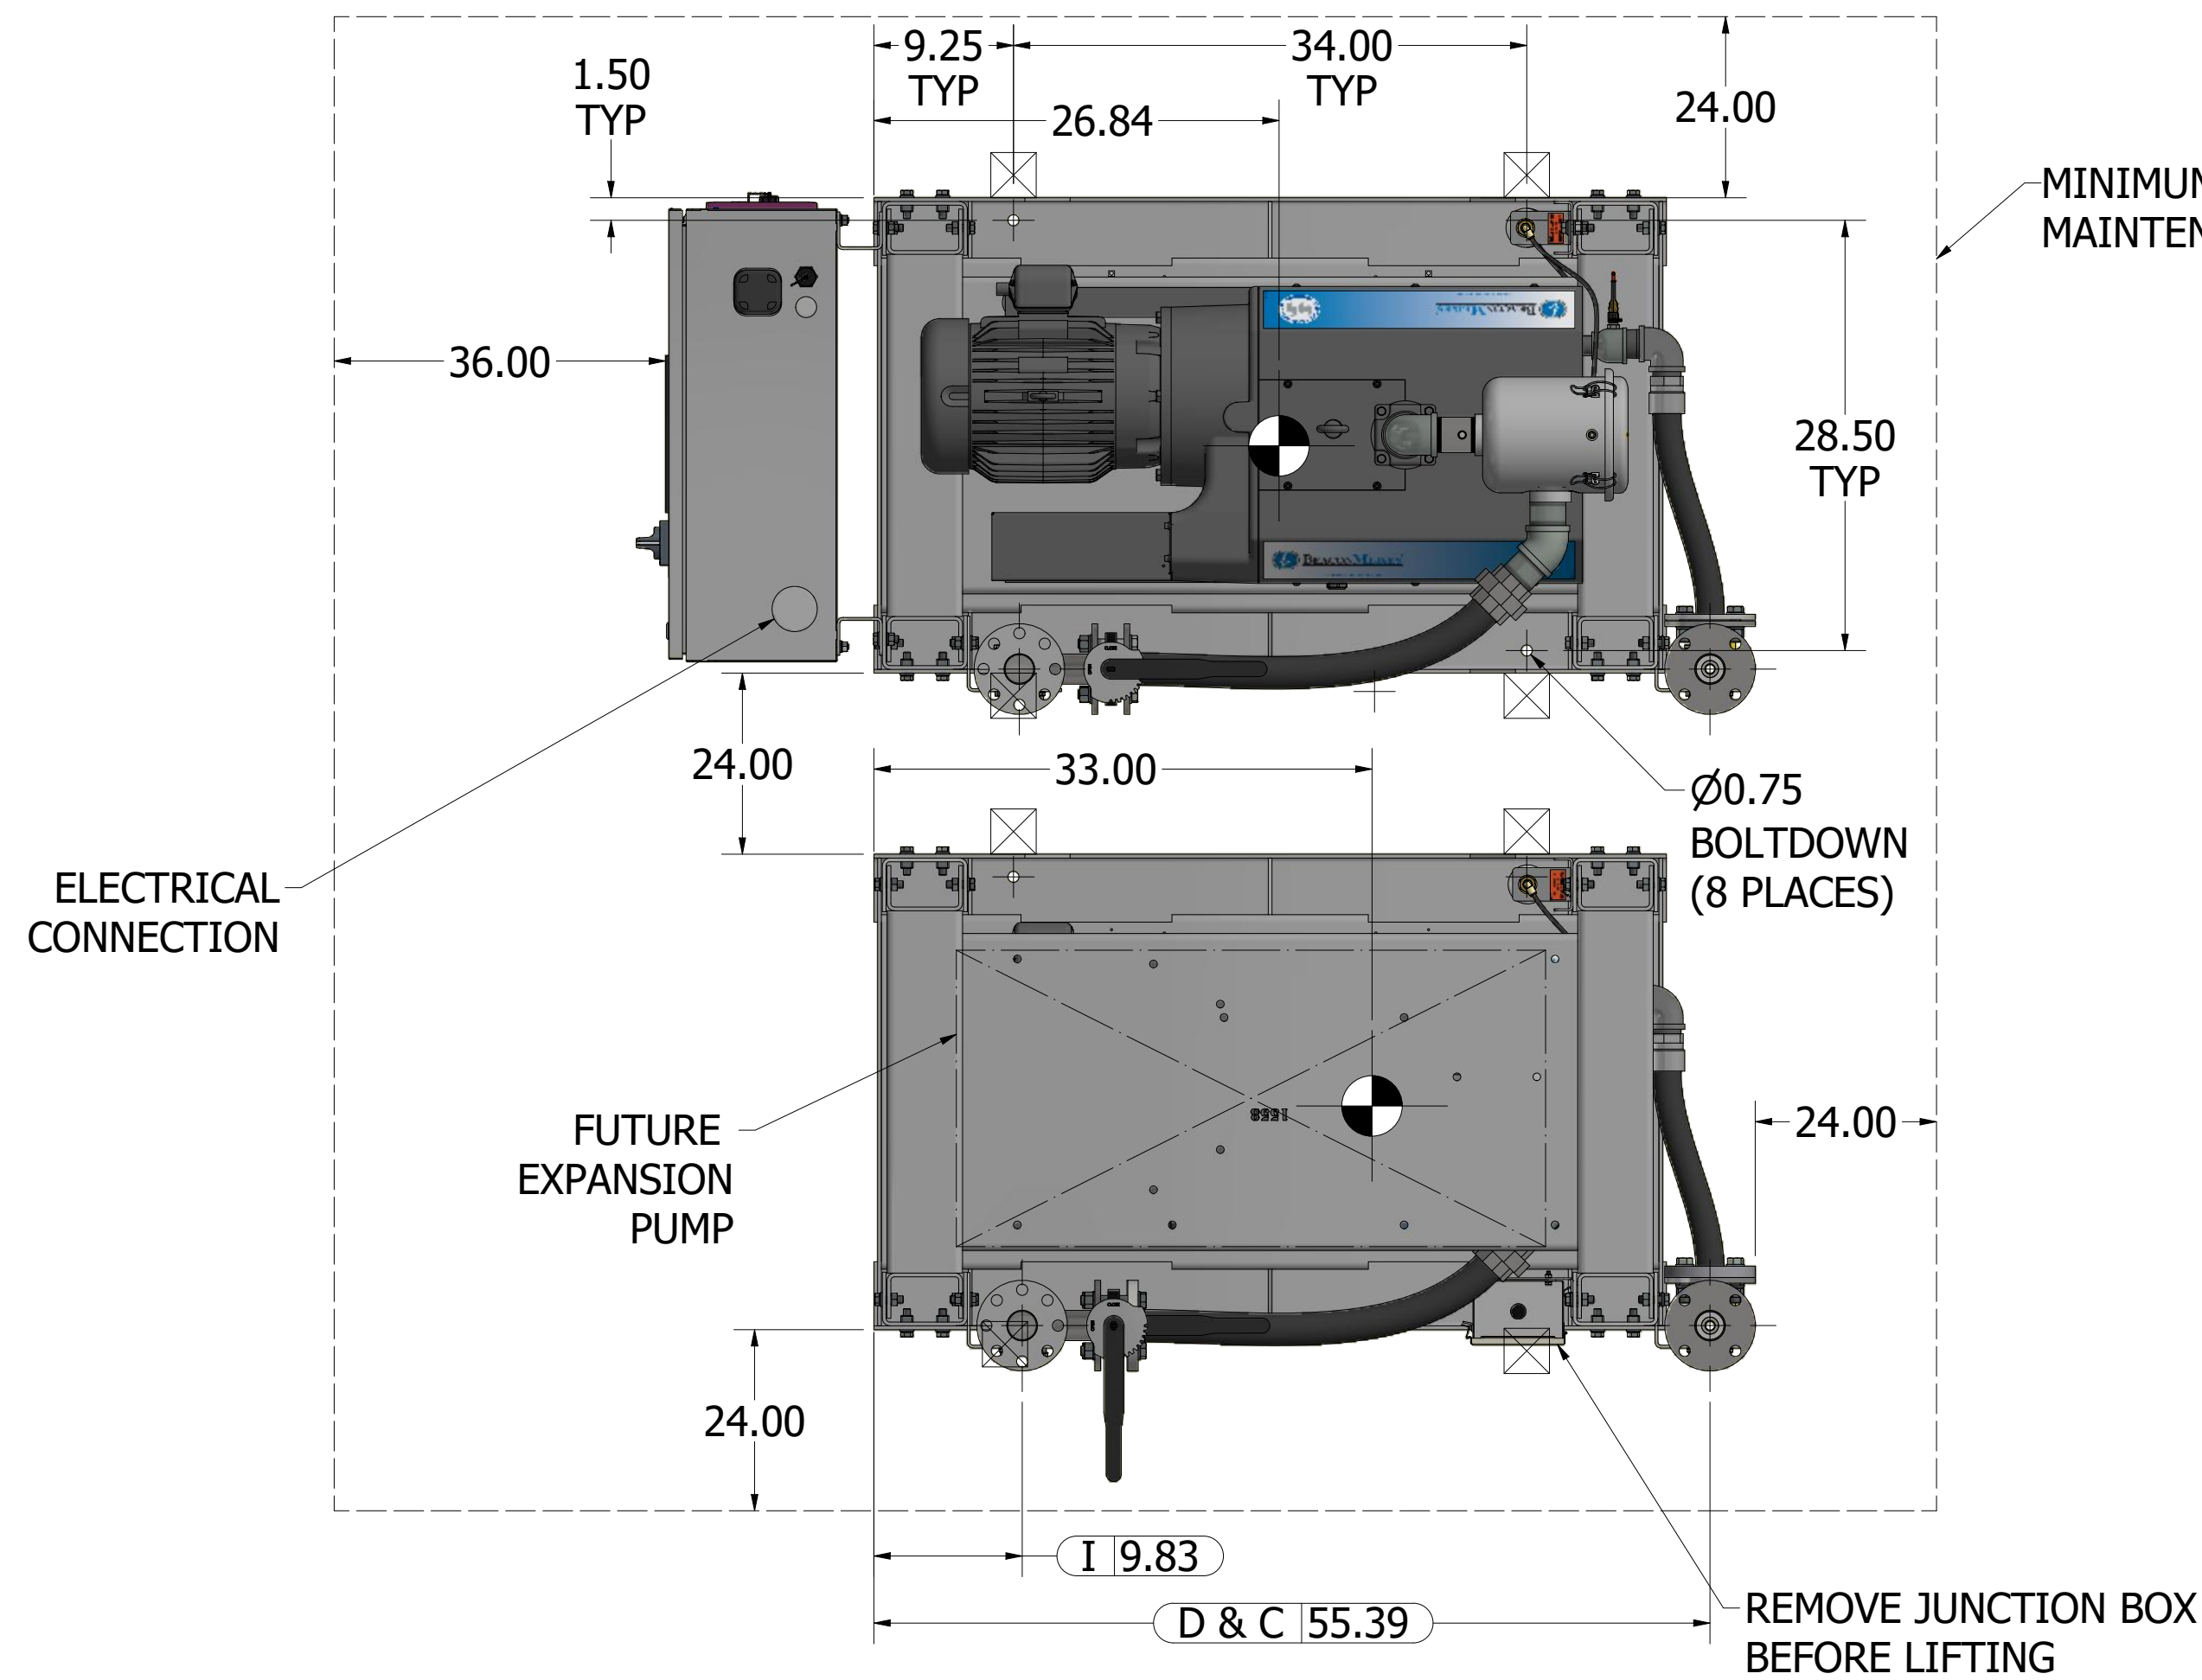

Revised:	LHG	Date:	11-23-2023	Drawn:	BJM	Date:	07-07-2024
 BEACON MEDICS		This drawing and the information contained therein remain the property of BeaconMedics and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedics Engineering.				Scale:	
Description:		Part Number:					
GENERAL ASSEMBLY 6.4HP TX-X-QX CLAW VSD VAC MOD 240G RECEIVER STANDARD AND O2 ASSURED		4107 8515 60 HOP230420				Rev:	03
		Sheet 1 of 1				DO NOT SCALE THIS DOCUMENT	