

NOTES:  
1. DISCHARGE MUFFLERS WILL BE SHIPPED LOOSE.

2. DX MODULE WEIGHT: 2,301 LBS.  
SX MODULE WEIGHT: 1,222 LBS  
240G TANK WEIGHT: 733 LBS  
CONTROL CABINET WEIGHT: 215 LBS.

3.  INDICATES LIFTING POINT.




4.  DENOTES CENTER OF GRAVITY.

SYSTEM CONNECTIONS	
ID	DESCRIPTION
I	INLET LOCATION
D	DISCHARGE LOCATION
C	CONDENSATE DRAIN LOCATION
T	TANK DRAIN LOCATION

REMOVE INTAKE MANIFOLD  
BEFORE LIFTING  
(3 PLACES)

REMOVE JUNCTION BOX  
BEFORE LIFTING  
(3 PLACES)

MINIMUM CLEARANCE FOR  
MAINTENANCE & VENTILATION

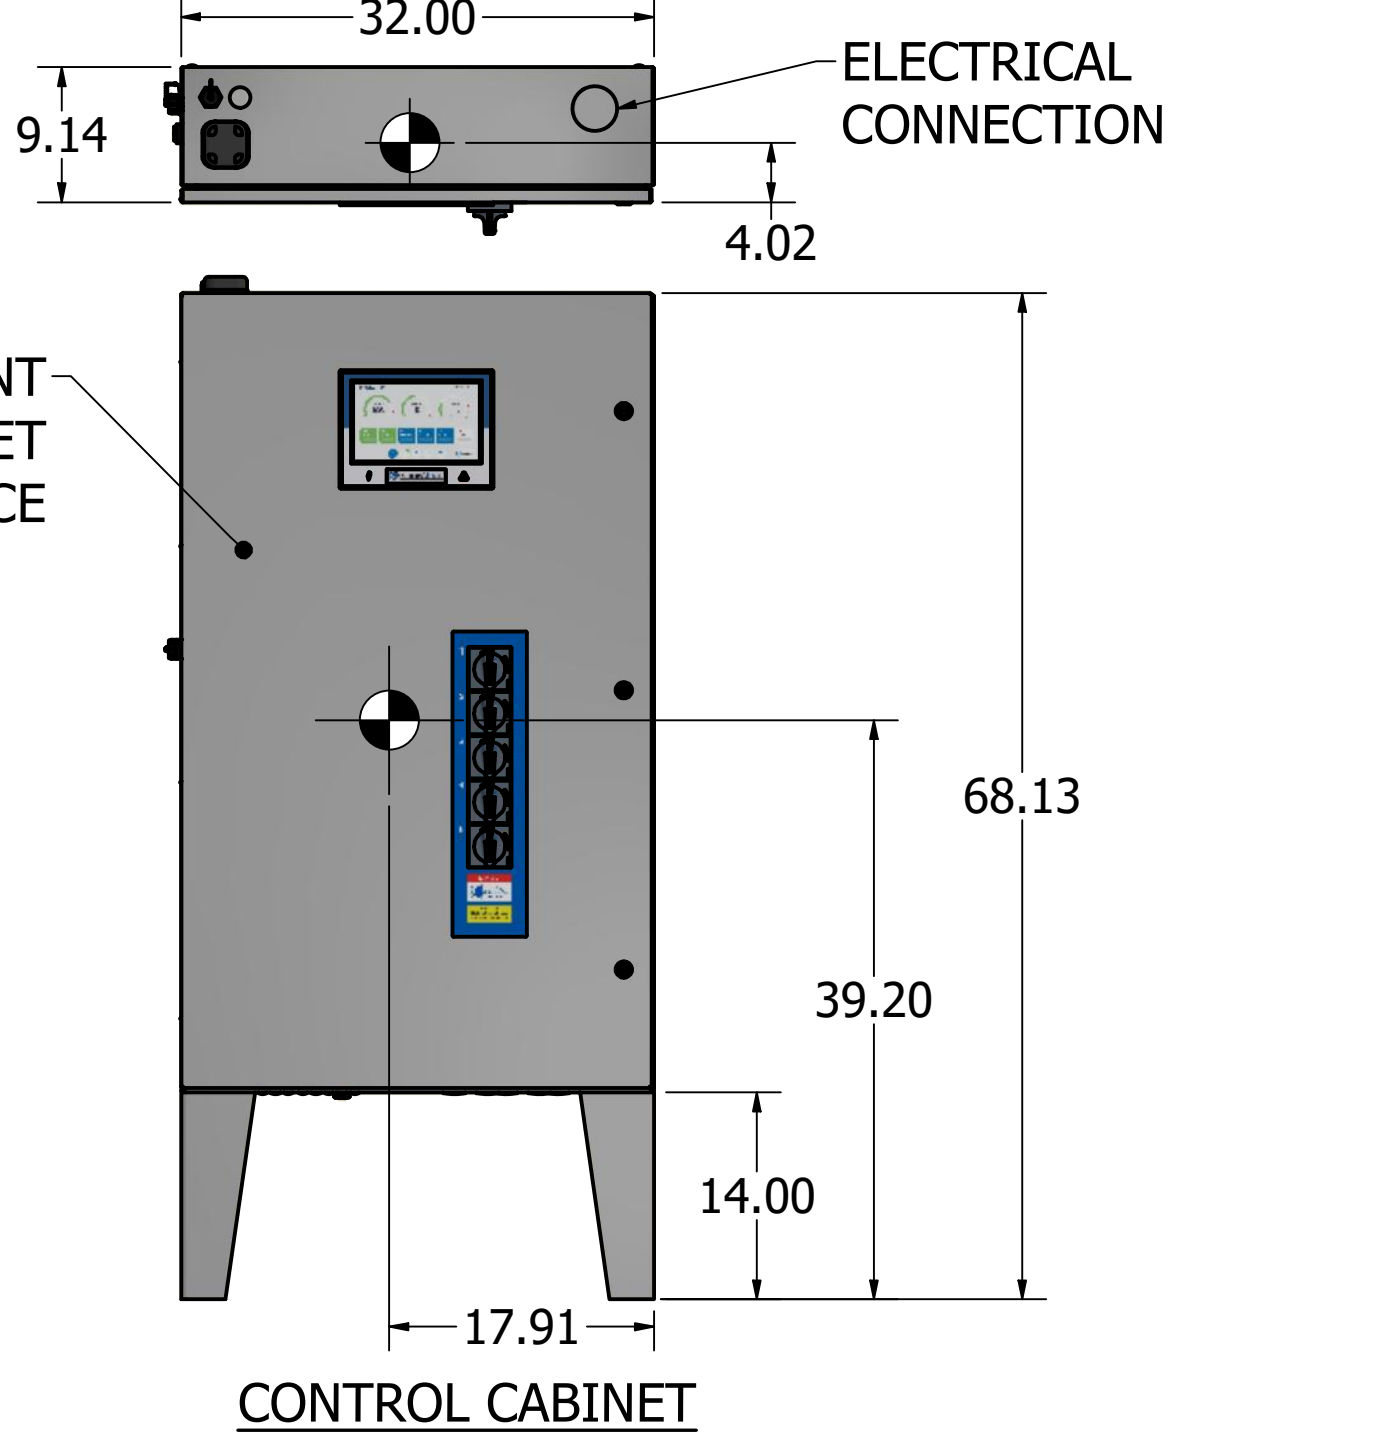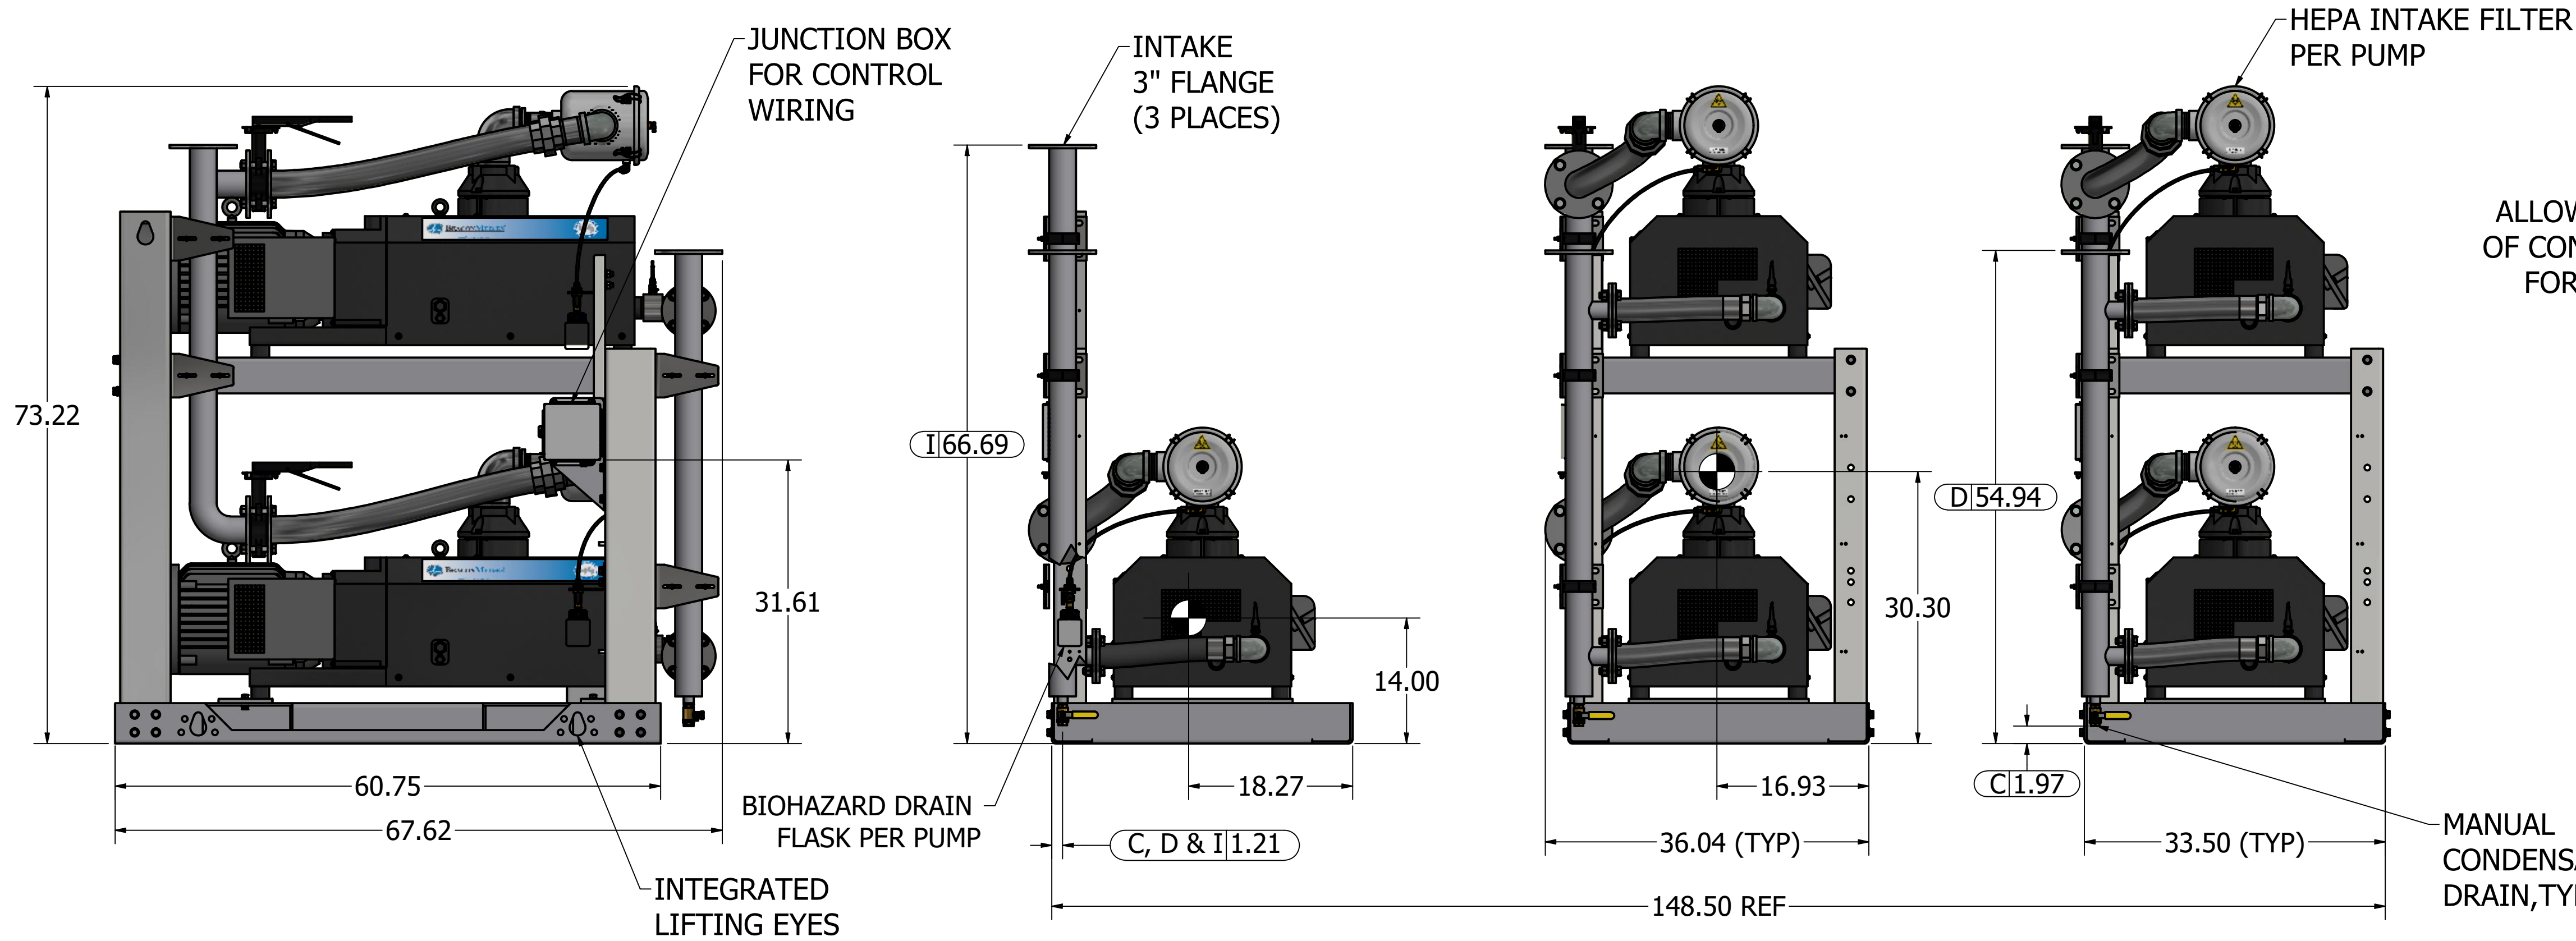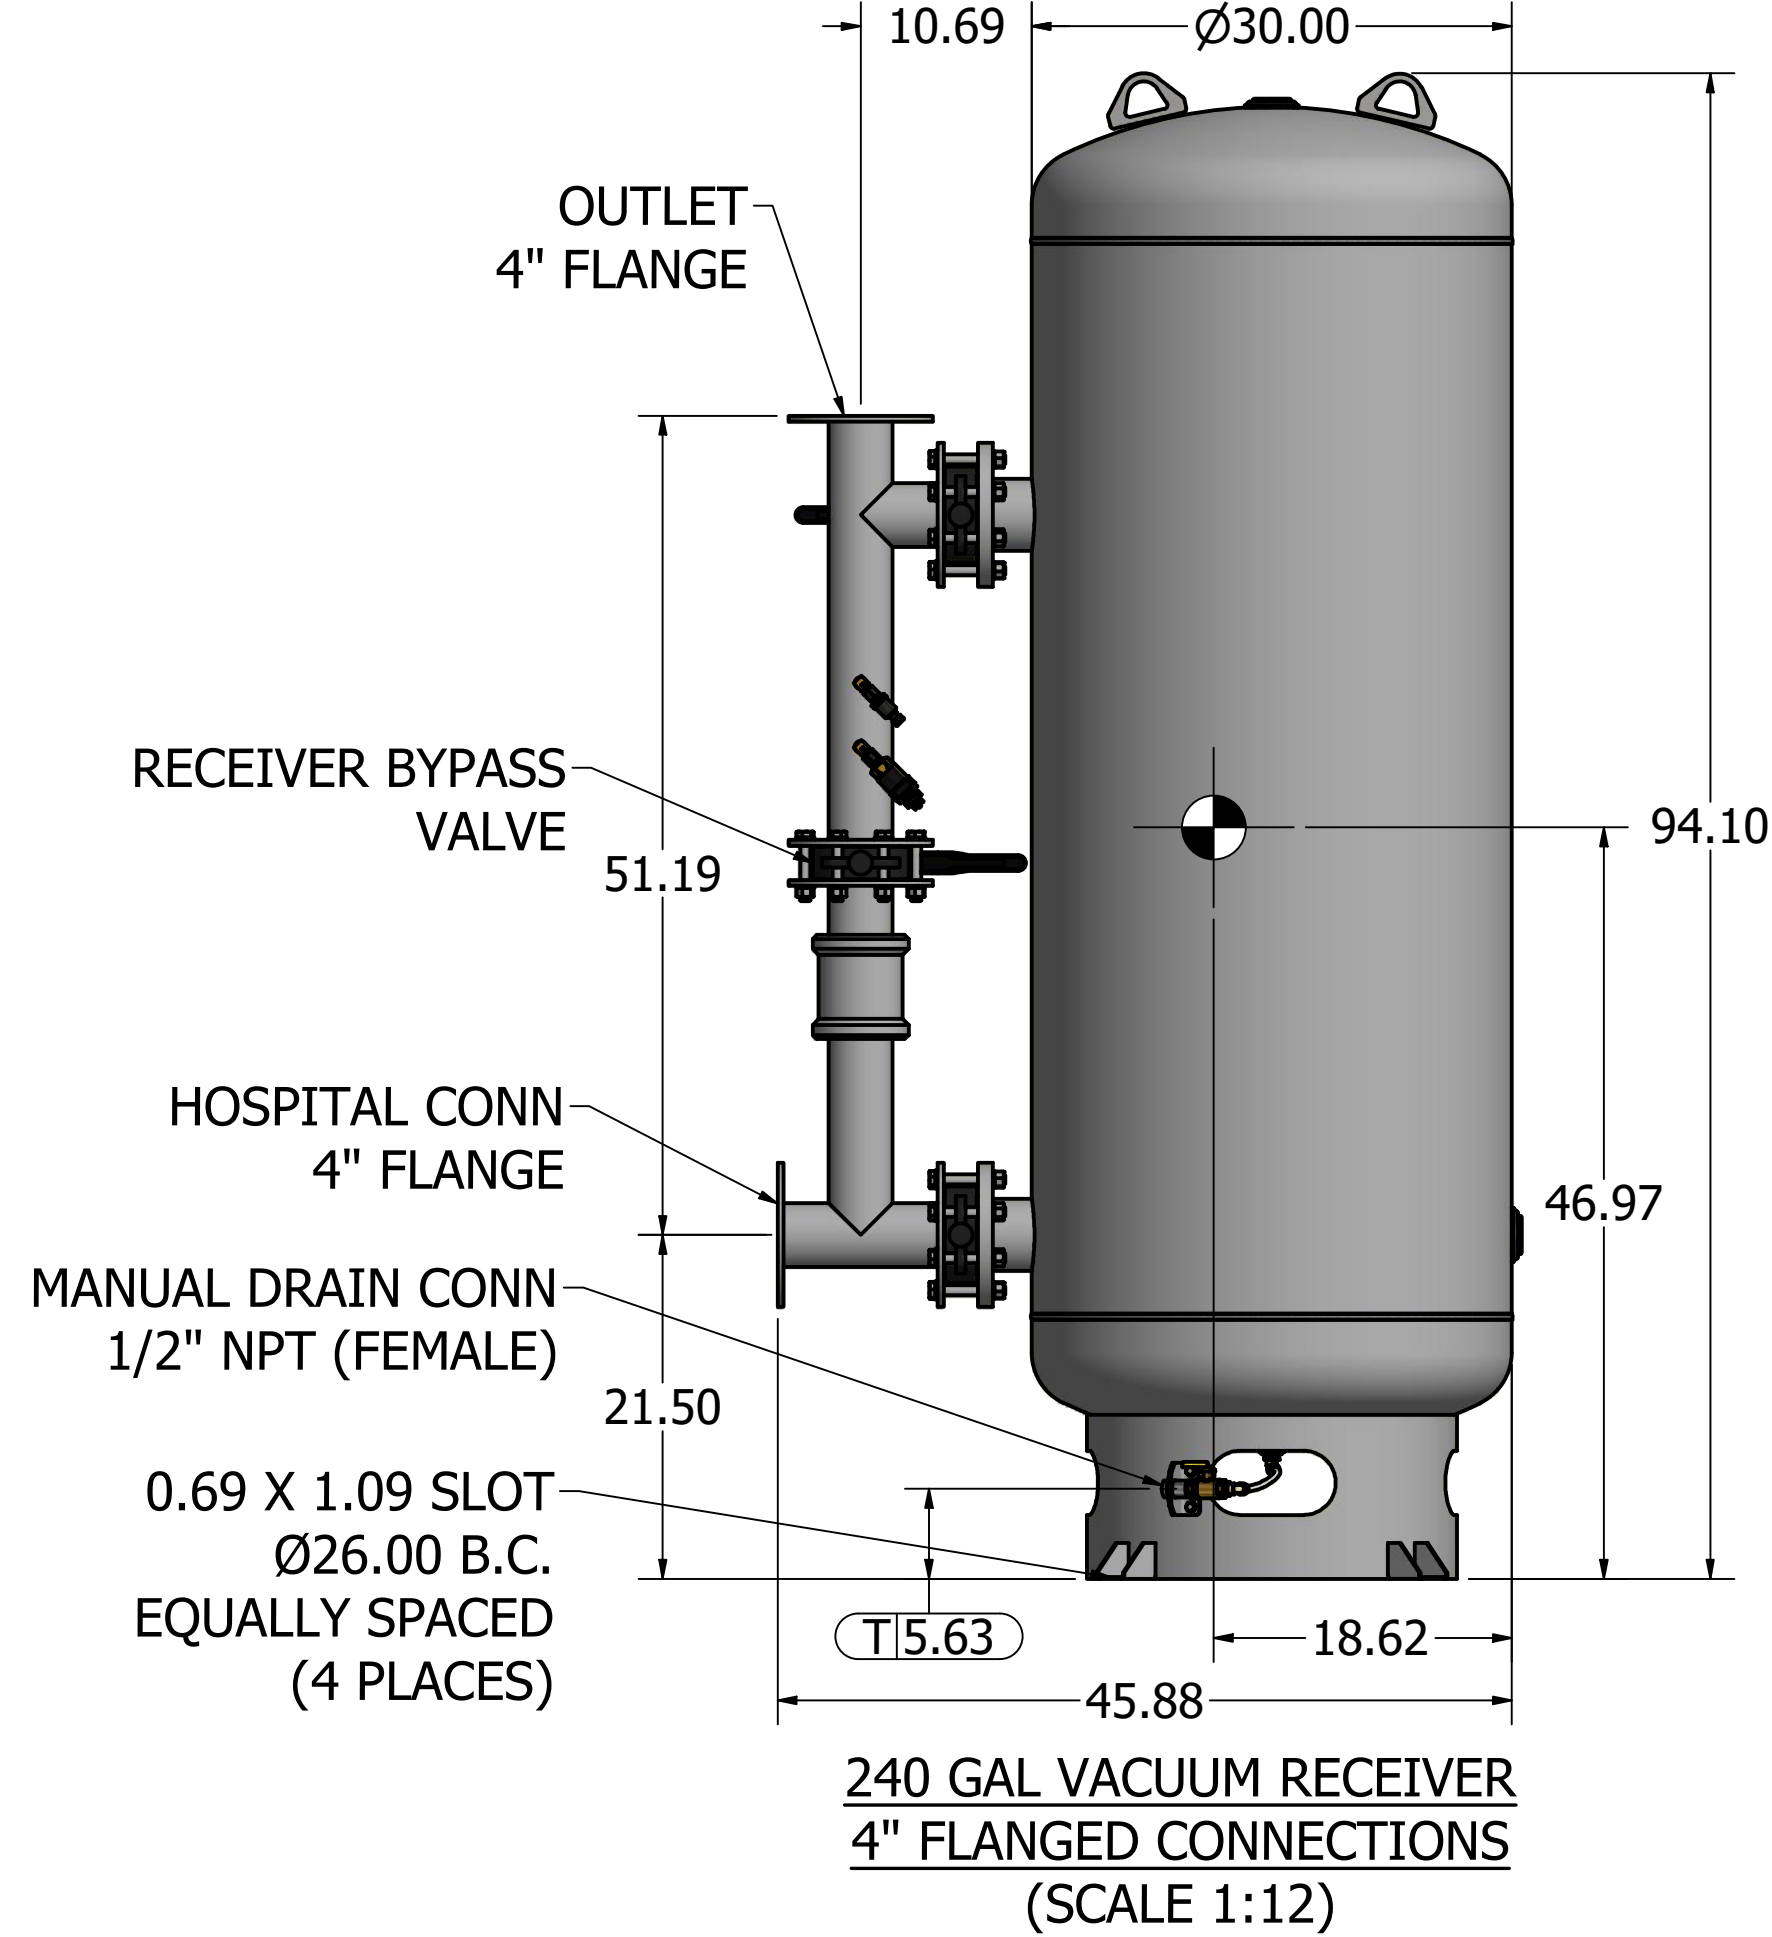

Revised: a00551998	Date: 4/11/2023	Drawn: JWO	Date: 2/7/2014
BEACONMED/ES		D	
Description: GENERAL ASSEMBLY 15HP PX CLAW VAC MOD 240G RECEIVER STANDARD		Part Number: 4107 8549 09	
DN: HOP230841		Rev: 03	
Sheet 1 of 1		DO NOT SCALE THIS DOCUMENT	