





Notes:

1. DX MODULE W/ PANEL WEIGHT: 1,478 LBS
DX MODULE WEIGHT: 1,312 LBS
200G TANK WEIGHT: 638 LBS
2.  INDICATES LIFTING POINT.
3.  DENOTES CENTER OF GRAVITY.


SYSTEM CONNECTIONS	
ID	DESCRIPTION
I	INLET LOCATION
D	DISCHARGE LOCATION
C	CONDENSATE DRAIN LOCATION
T	TANK DRAIN

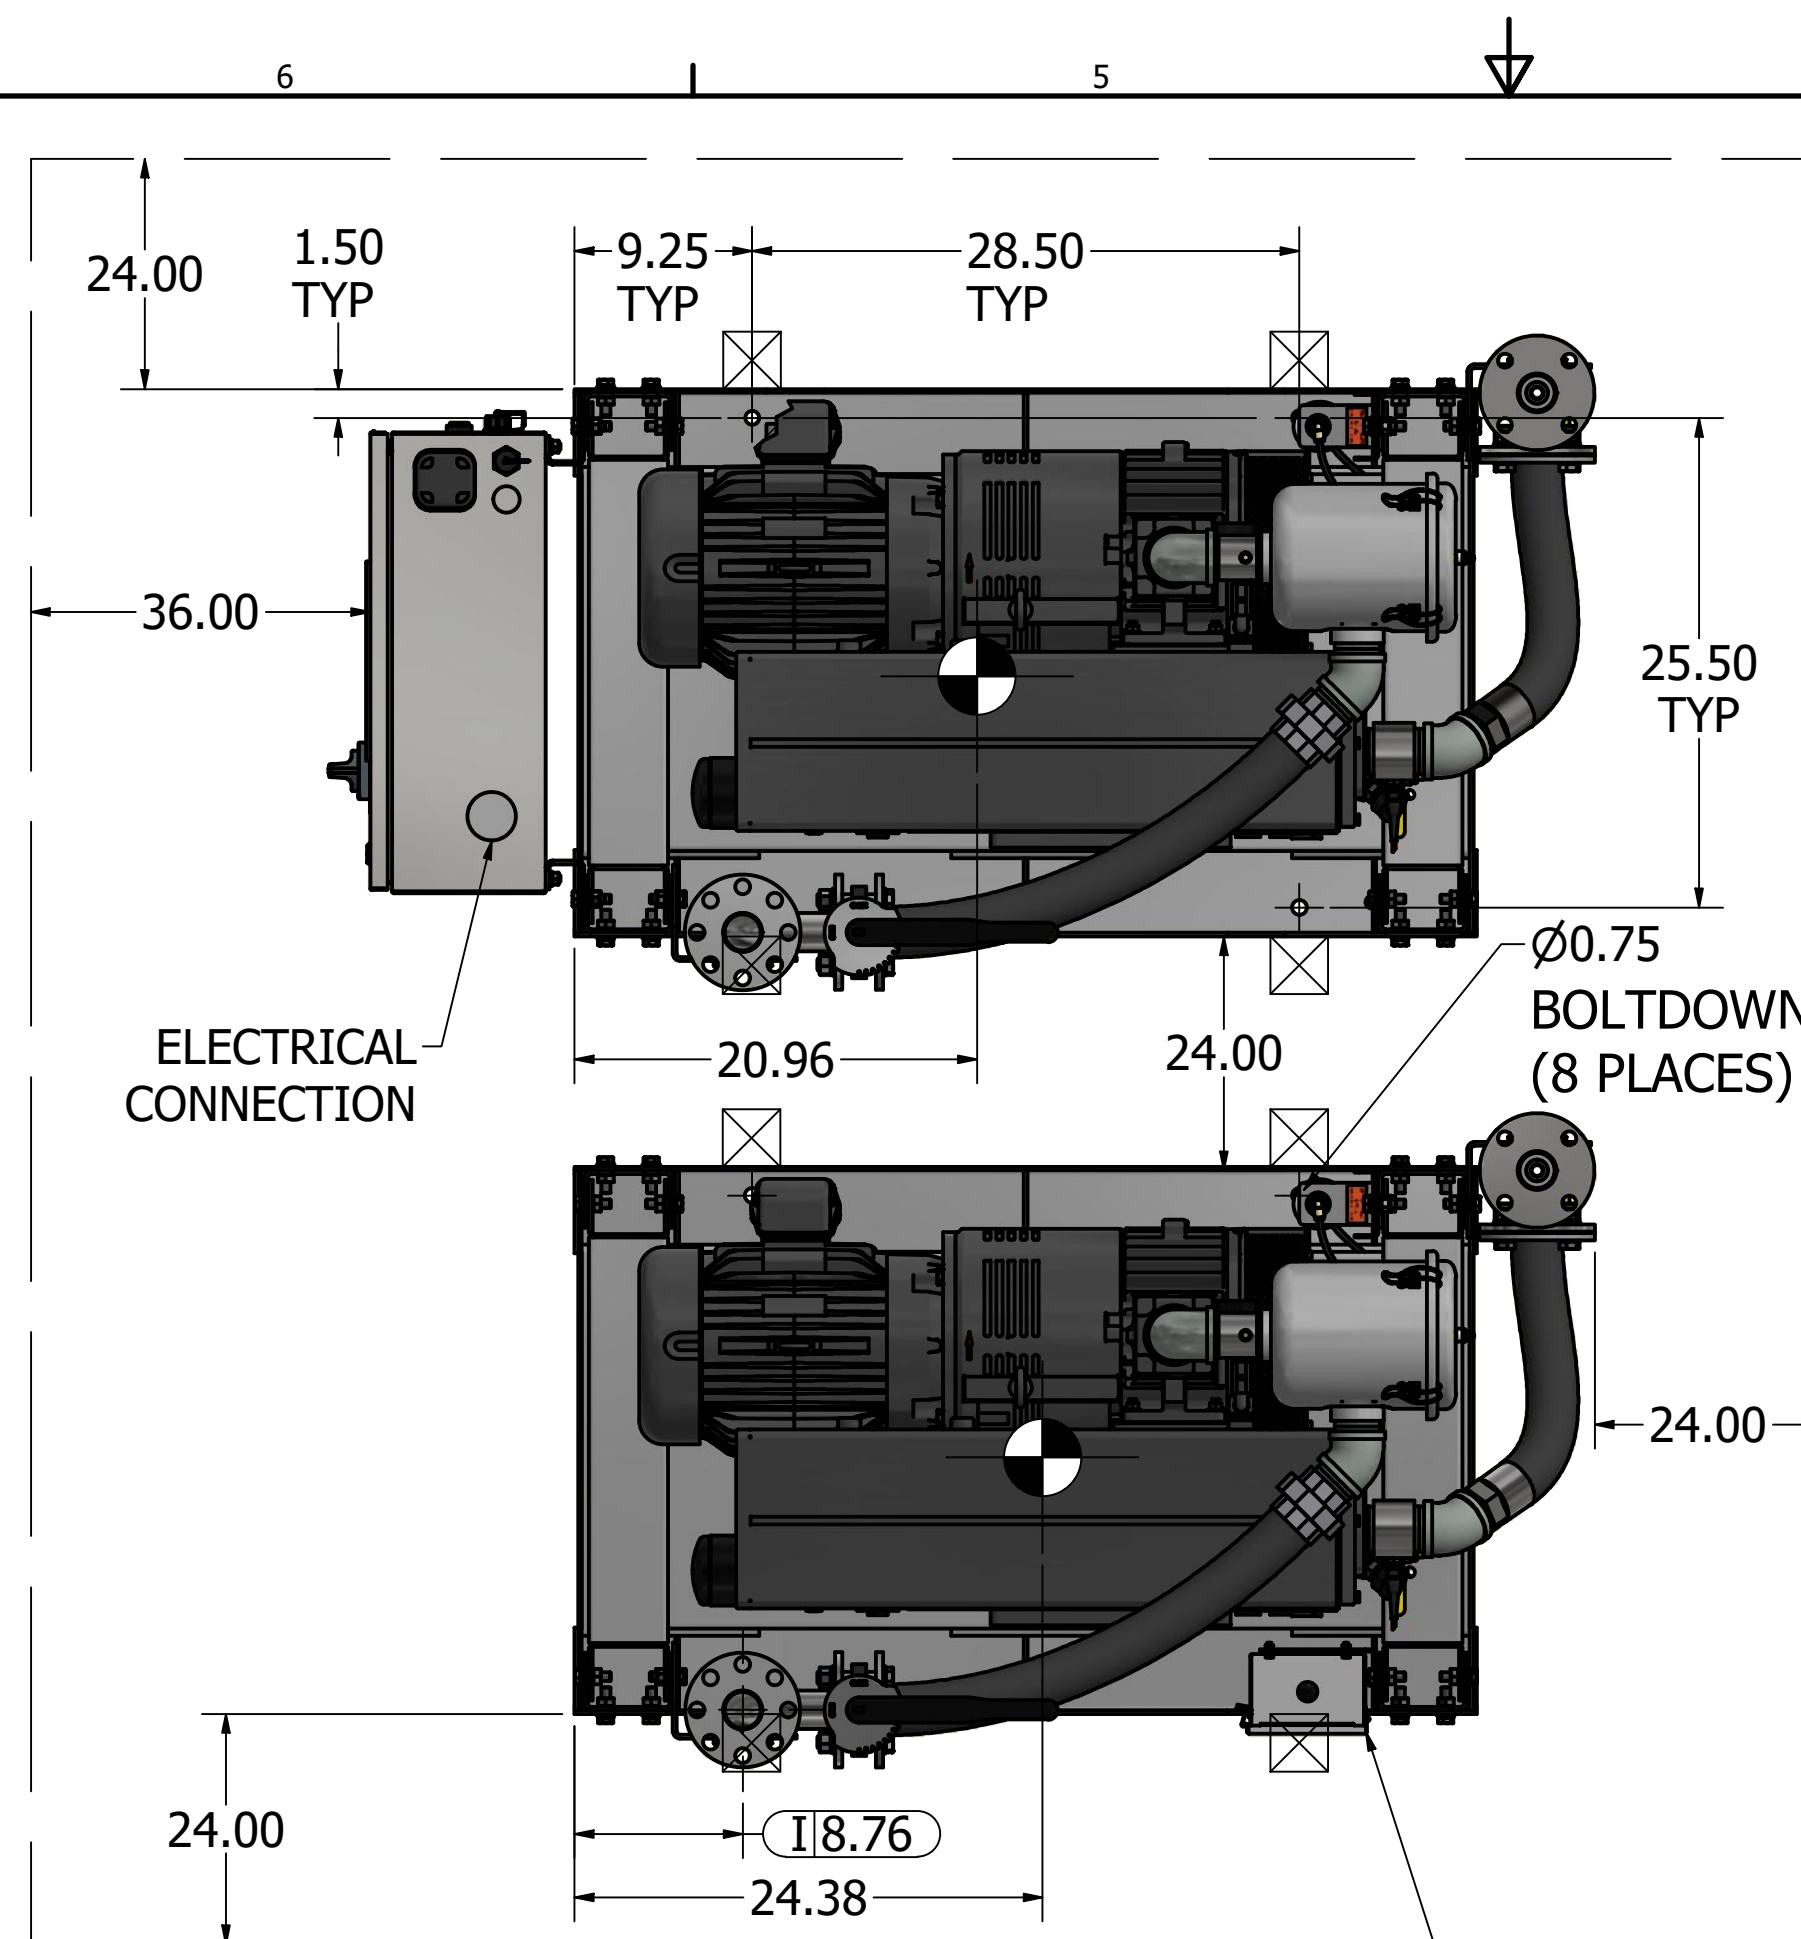


MINIMUM CLEARANCE FOR
MAINTENANCE & VENTILATION

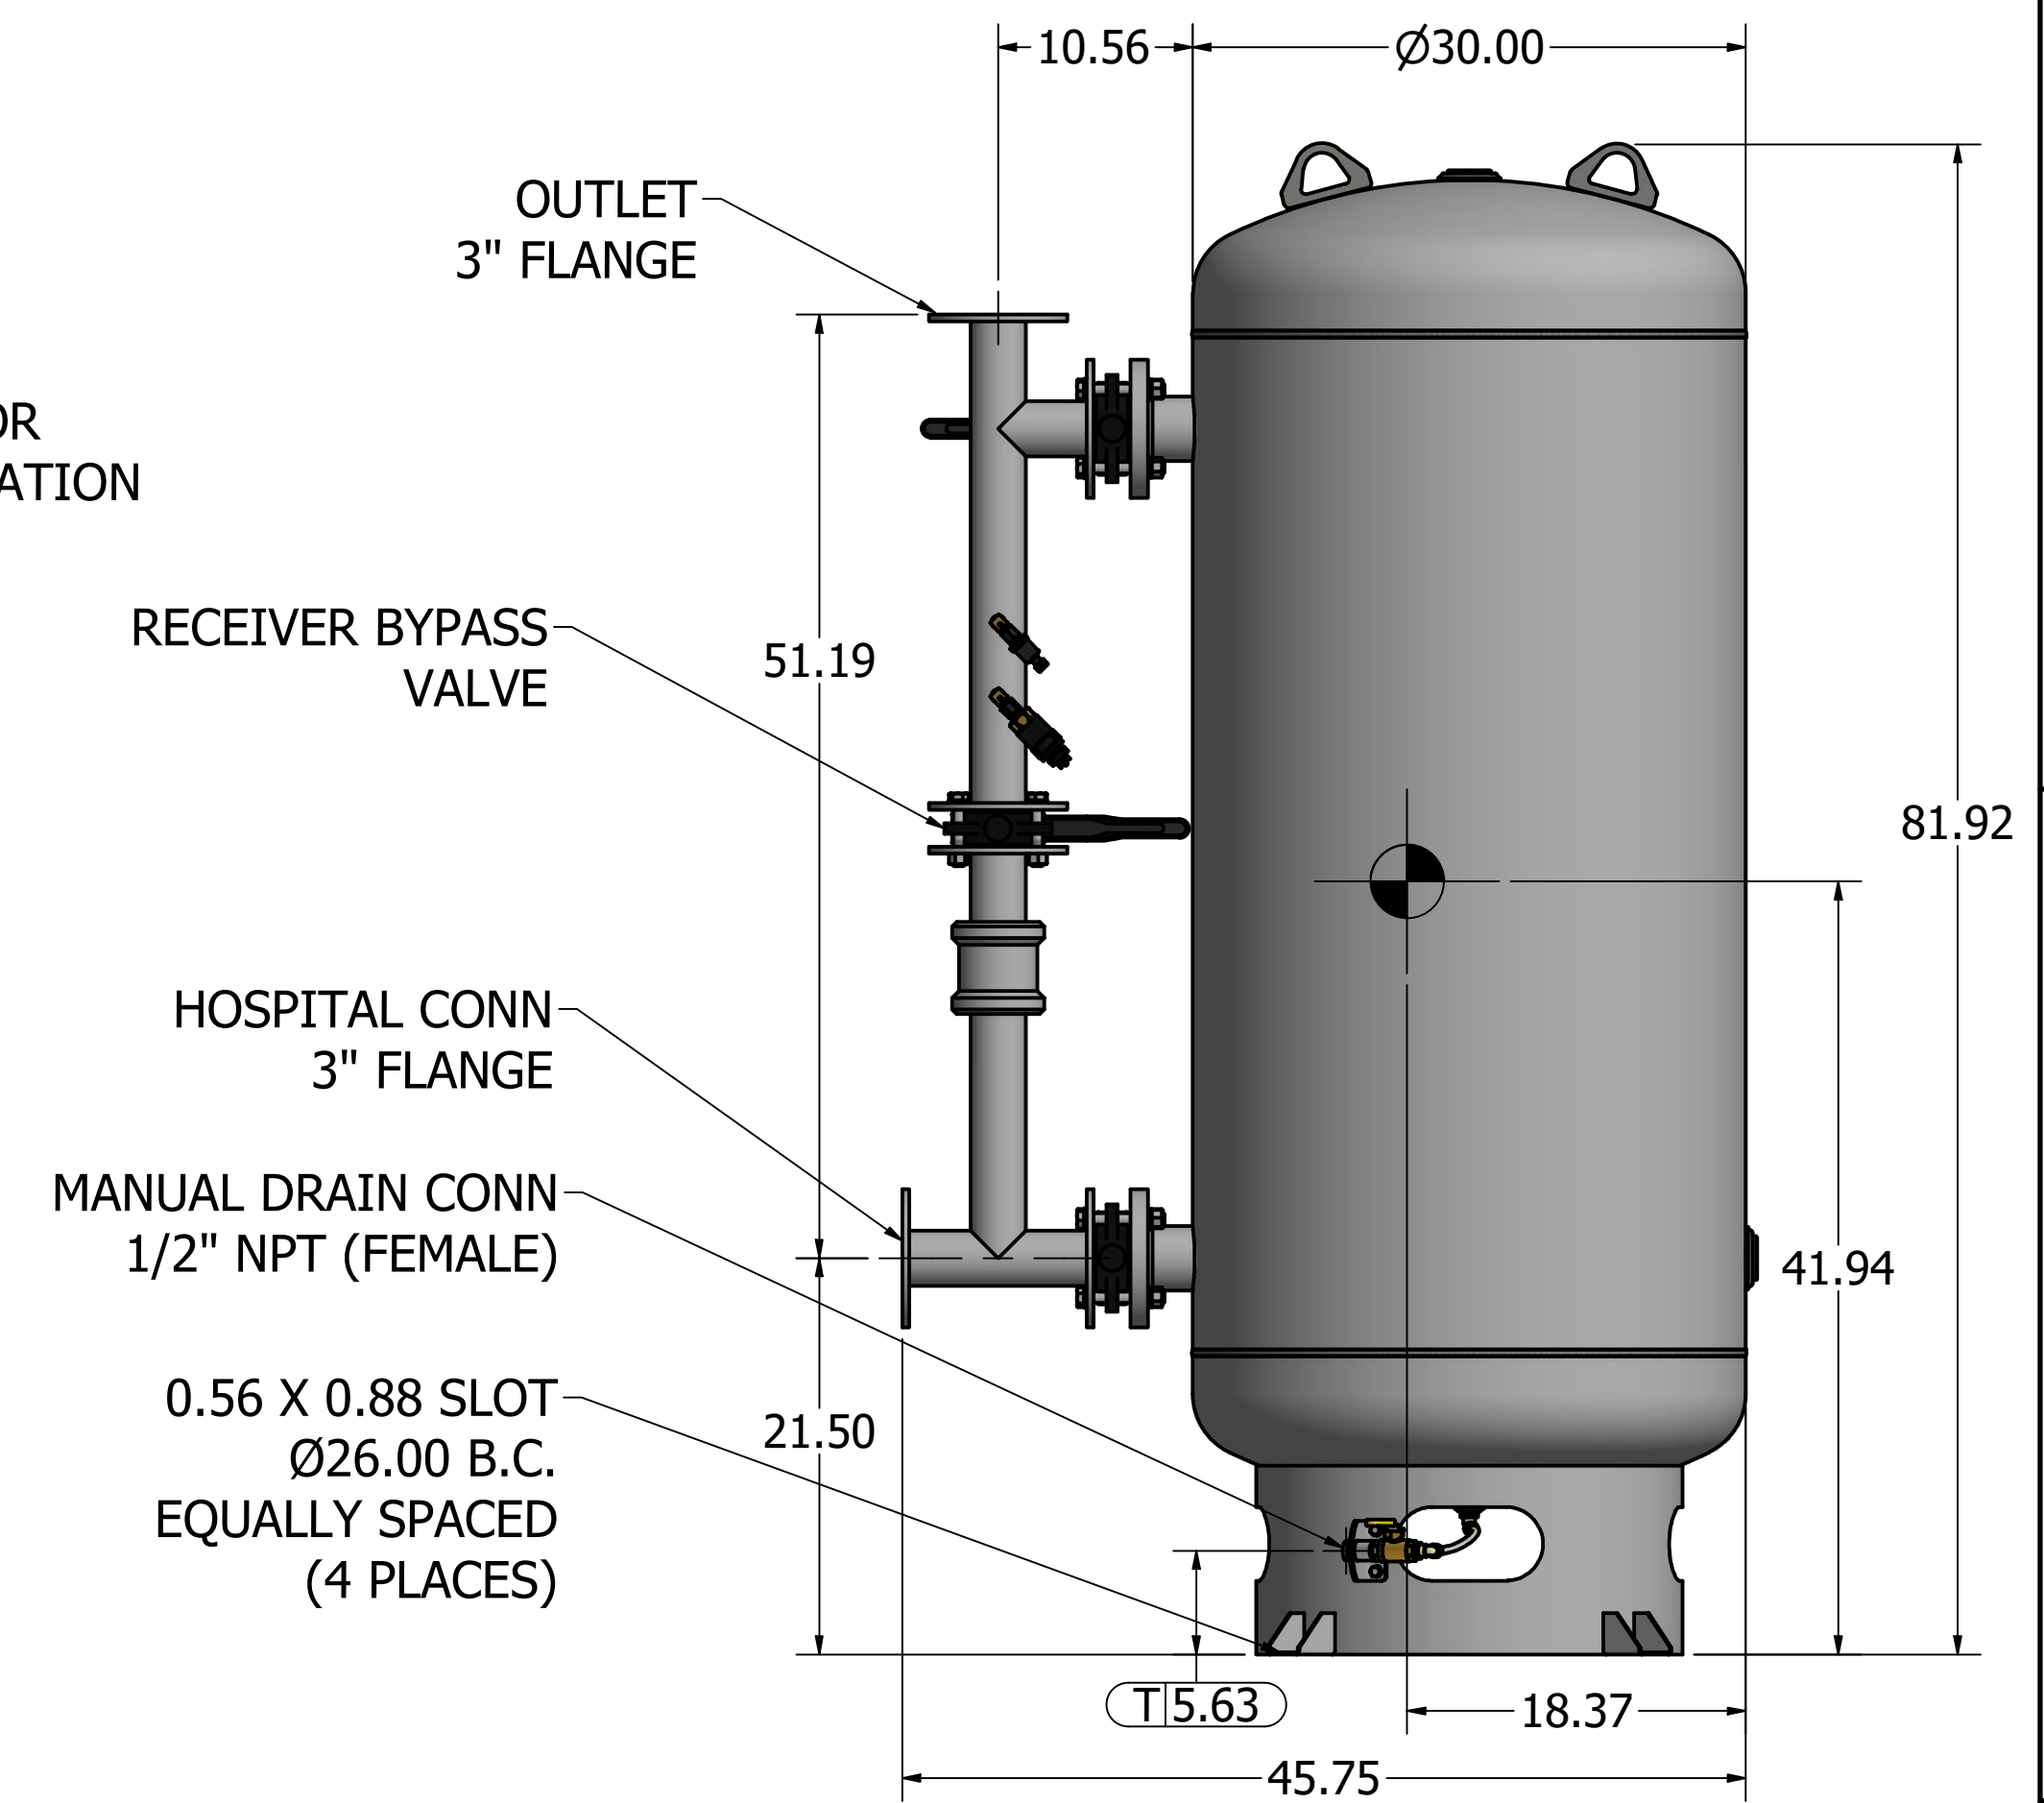

200 GAL VACUUM RECEIVER
3" FLANGED CONNECTIONS
(SCALE 1:10)

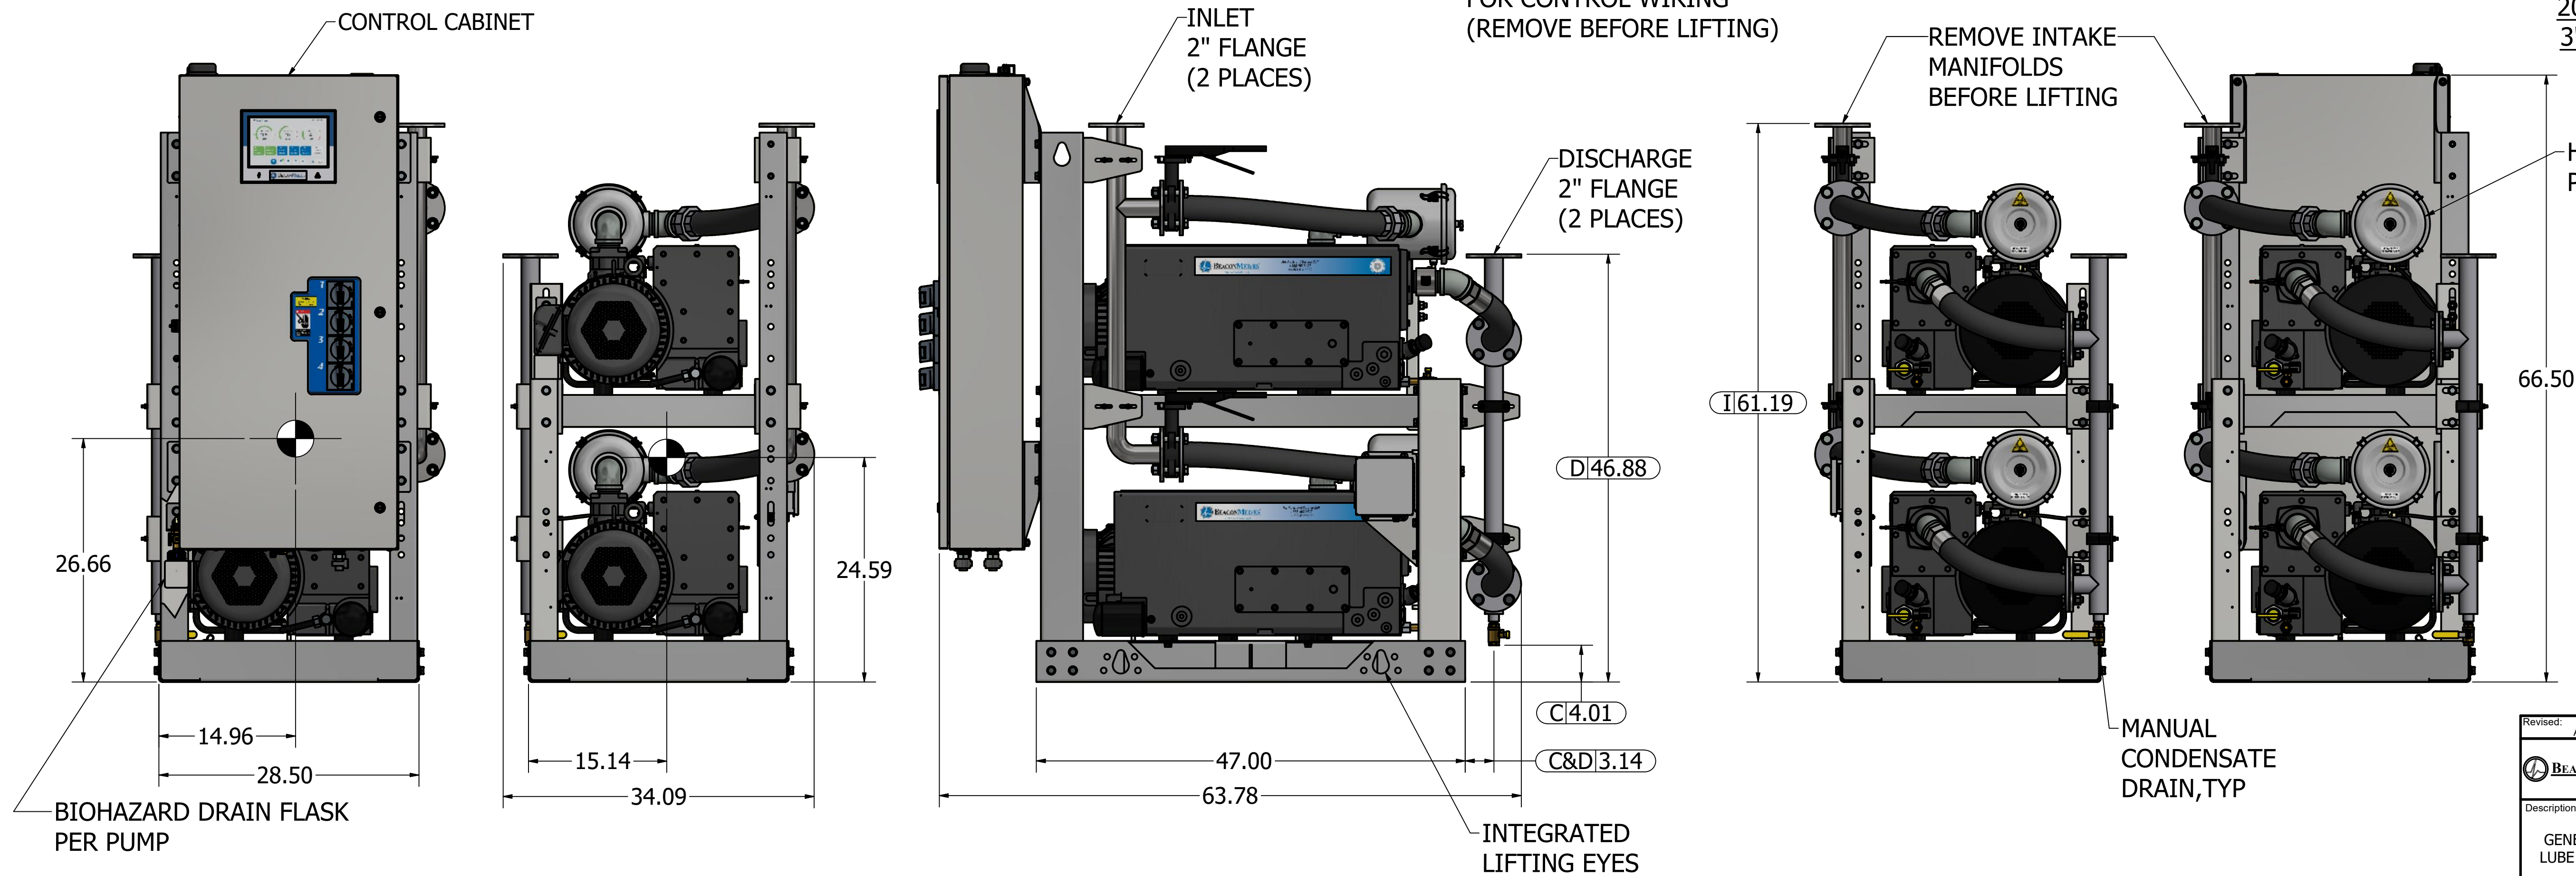

Revised: APS		Date: 3/24/2023	Drawn: USNKNW	Date: 10/26/2010
 BEACONMEDICS		This drawing and the information contained thereon remain the property of BeaconMedics and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedics Engineering.		Scale:
				D
Description:		Part Number: 4107 8522 23		
GENERAL ASSEMBLY 7.5HP QX LUBE VAC MOD 200G RECEIVER		DN: HOP230842		Rev: 03
		Sheet 1 of 1		DO NOT SCALE THIS DOCUMENT