
NOTES:


- 1. ALL INTERCONNECTING PIPE AND FITTINGS SHALL BE INSTALLED BY THE CONTRACTOR.
- D 2. PIPING LAYOUT IS DIAGRAMMATIC ONLY. FINAL ARRANGEMENT WILL BE SITE SPECIFIC. CONTRACTOR WILL BE RESPONSIBLE FOR FIELD VERIFICATION AND COORDINATING ACTUAL LOCATION WITH ALL OTHER TRADES.
- 3. CONTRACTOR SHALL VERIFY MOTOR VOLTAGE, PHASE AND AMP RATINGS BEFORE STARTING ELECTRICAL INSTALLATION: AND MAKE CERTAIN THE VOLTAGE SUPPLIED BY THE FACILITY IS THE SAME.
- 4. THE ROOM REQUIRES DEDICATED MECHANICAL VENTILATION WITH AN ALLOWABLE TEMPERATURE VARIANCE OF 40° TO 105°F. (FOR HIGHER AMBIENTS, CONSULT FACTORY)
- 5. ALL ACCESSORIES, PIPE AND FITTINGS, EXCEPT DISCHARGE SILENCERS, BEYOND INLET AND DISCHARGE PORTS ARE SUPPLIED AND INSTALLED BY OTHERS.
- 6. ALLOW 36 INCHES IN FRONT OF CONTROL PANEL FOR MAINTENANCE AND VENTILATION. ALL OTHER SIDES REQUIRE 24 INCHES OF CLEARANCE.
- 7. WHEN DETERMINING THE TOTAL PIPE LENGTH, AND ALL THE STRAIGHT LENGTHS OF PIPE TOGETHER IN ADDITION TO THE NUMBER OF ELBOWS TIMES THE EFFECTIVE PIPE LENGTH FOR THAT PIPE SIZE. (SEE EQUIVALENT PIPE LENGTH TABLE & EXAMPLE CALCULATION IN THE O&M MANUAL)

EXHAUST PIPE SIZE TABLE (SEE NOTE 7)				
UNIT SIZE	PIPE LENGTH			
DX 15	0-50'	51'-450'	451'-500'	
	3.00 NPT	4.00 NPT	5.00 NPT	
UNIT SIZE	PIPE LENGTH			
DX 20	0-250'		251'-500'	
	4.00 NPT		5.00 NPT	
UNIT SIZE	PIPE LENGTH			
DX 25	0-150'		151'-500'	
	4.00 NPT		5.00 NPT	

EFFECTIVE PIPE LENGTH					
FOR ELBOWS					
PIPE SIZE (IN)	3.00" NPT	4.00" NPT	5.00" NPT		
EFF. PIPE LENGTH (FT)	7.9	10	11.9		

— — FIELD PIPING INLET ====FIELD PIPING OUTLET

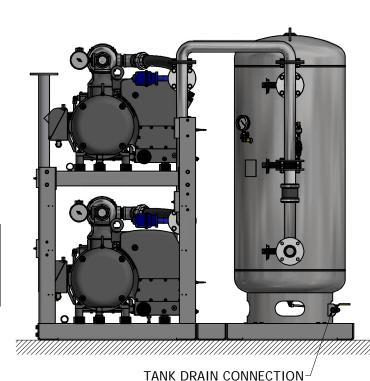

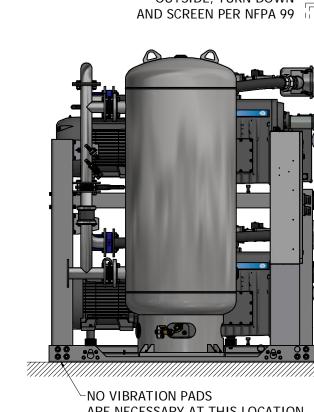

DRIP LEG VALVE ARE NECESSARY AT THIS LOCATION

PIPE EXHAUST

OUTSIDE, TURN DOWN

SOURCE SHUTOFF VALVE ┌INLET 3" FLANGE

-MAIN LINE VACUUM SWITCH

-MAIN VACUUM GAUGE

FROM LABORATORY-

ETHERNET WIRING ACCESS

-DISCHARGE 3" FLANGE

ALARM WIRING ACCESS-

FOR INTAKE PIPE SIZING REFER TO STANDARD-

PRESSURE DROP TABLES. TOTAL PRESSURE

DROP SHOULD BE LESS THAN 2" Hg AT A SYSTEM VACUUM LEVEL OF 15" Hg.

> SINGLE POINT POWER WIRING ACCESS

NO FOUNDATION OR INERTIA PAD IS REQUIRED (HOUSEKEEPING PAD IS OPTIONAL)

> 4107 8563 24 INSTALLATION DIAGRAM LAB BM190347 15-25HP DX LUBE VAC SPC heet 1 of 1

(25HP WITH 200 GALLON RECEIVER SHOWN)