




Notes:

1. SYSTEM WEIGHT: 8,650 LBS.
(INCLUDES FUTURE EXPANSION PUMP)
2.  INDICATES LIFTING POINT.
3.  DENOTES CENTER OF GRAVITY.
(INCLUDES FUTURE EXPANSION PUMP)


SYSTEM CONNECTIONS	
ID	DESCRIPTION
I	INLET LOCATION
D	DISCHARGE LOCATION
C	CONDENSATE DRAIN LOCATION
T	TANK DRAIN LOCATION

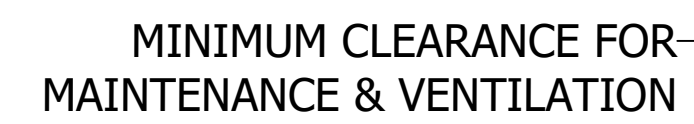

FUTURE-
EXPANSION
PUMP

ELECTRICAL-
CONNECTION

—Ø0.75
BOLTDOWNS
(12 PLACES)

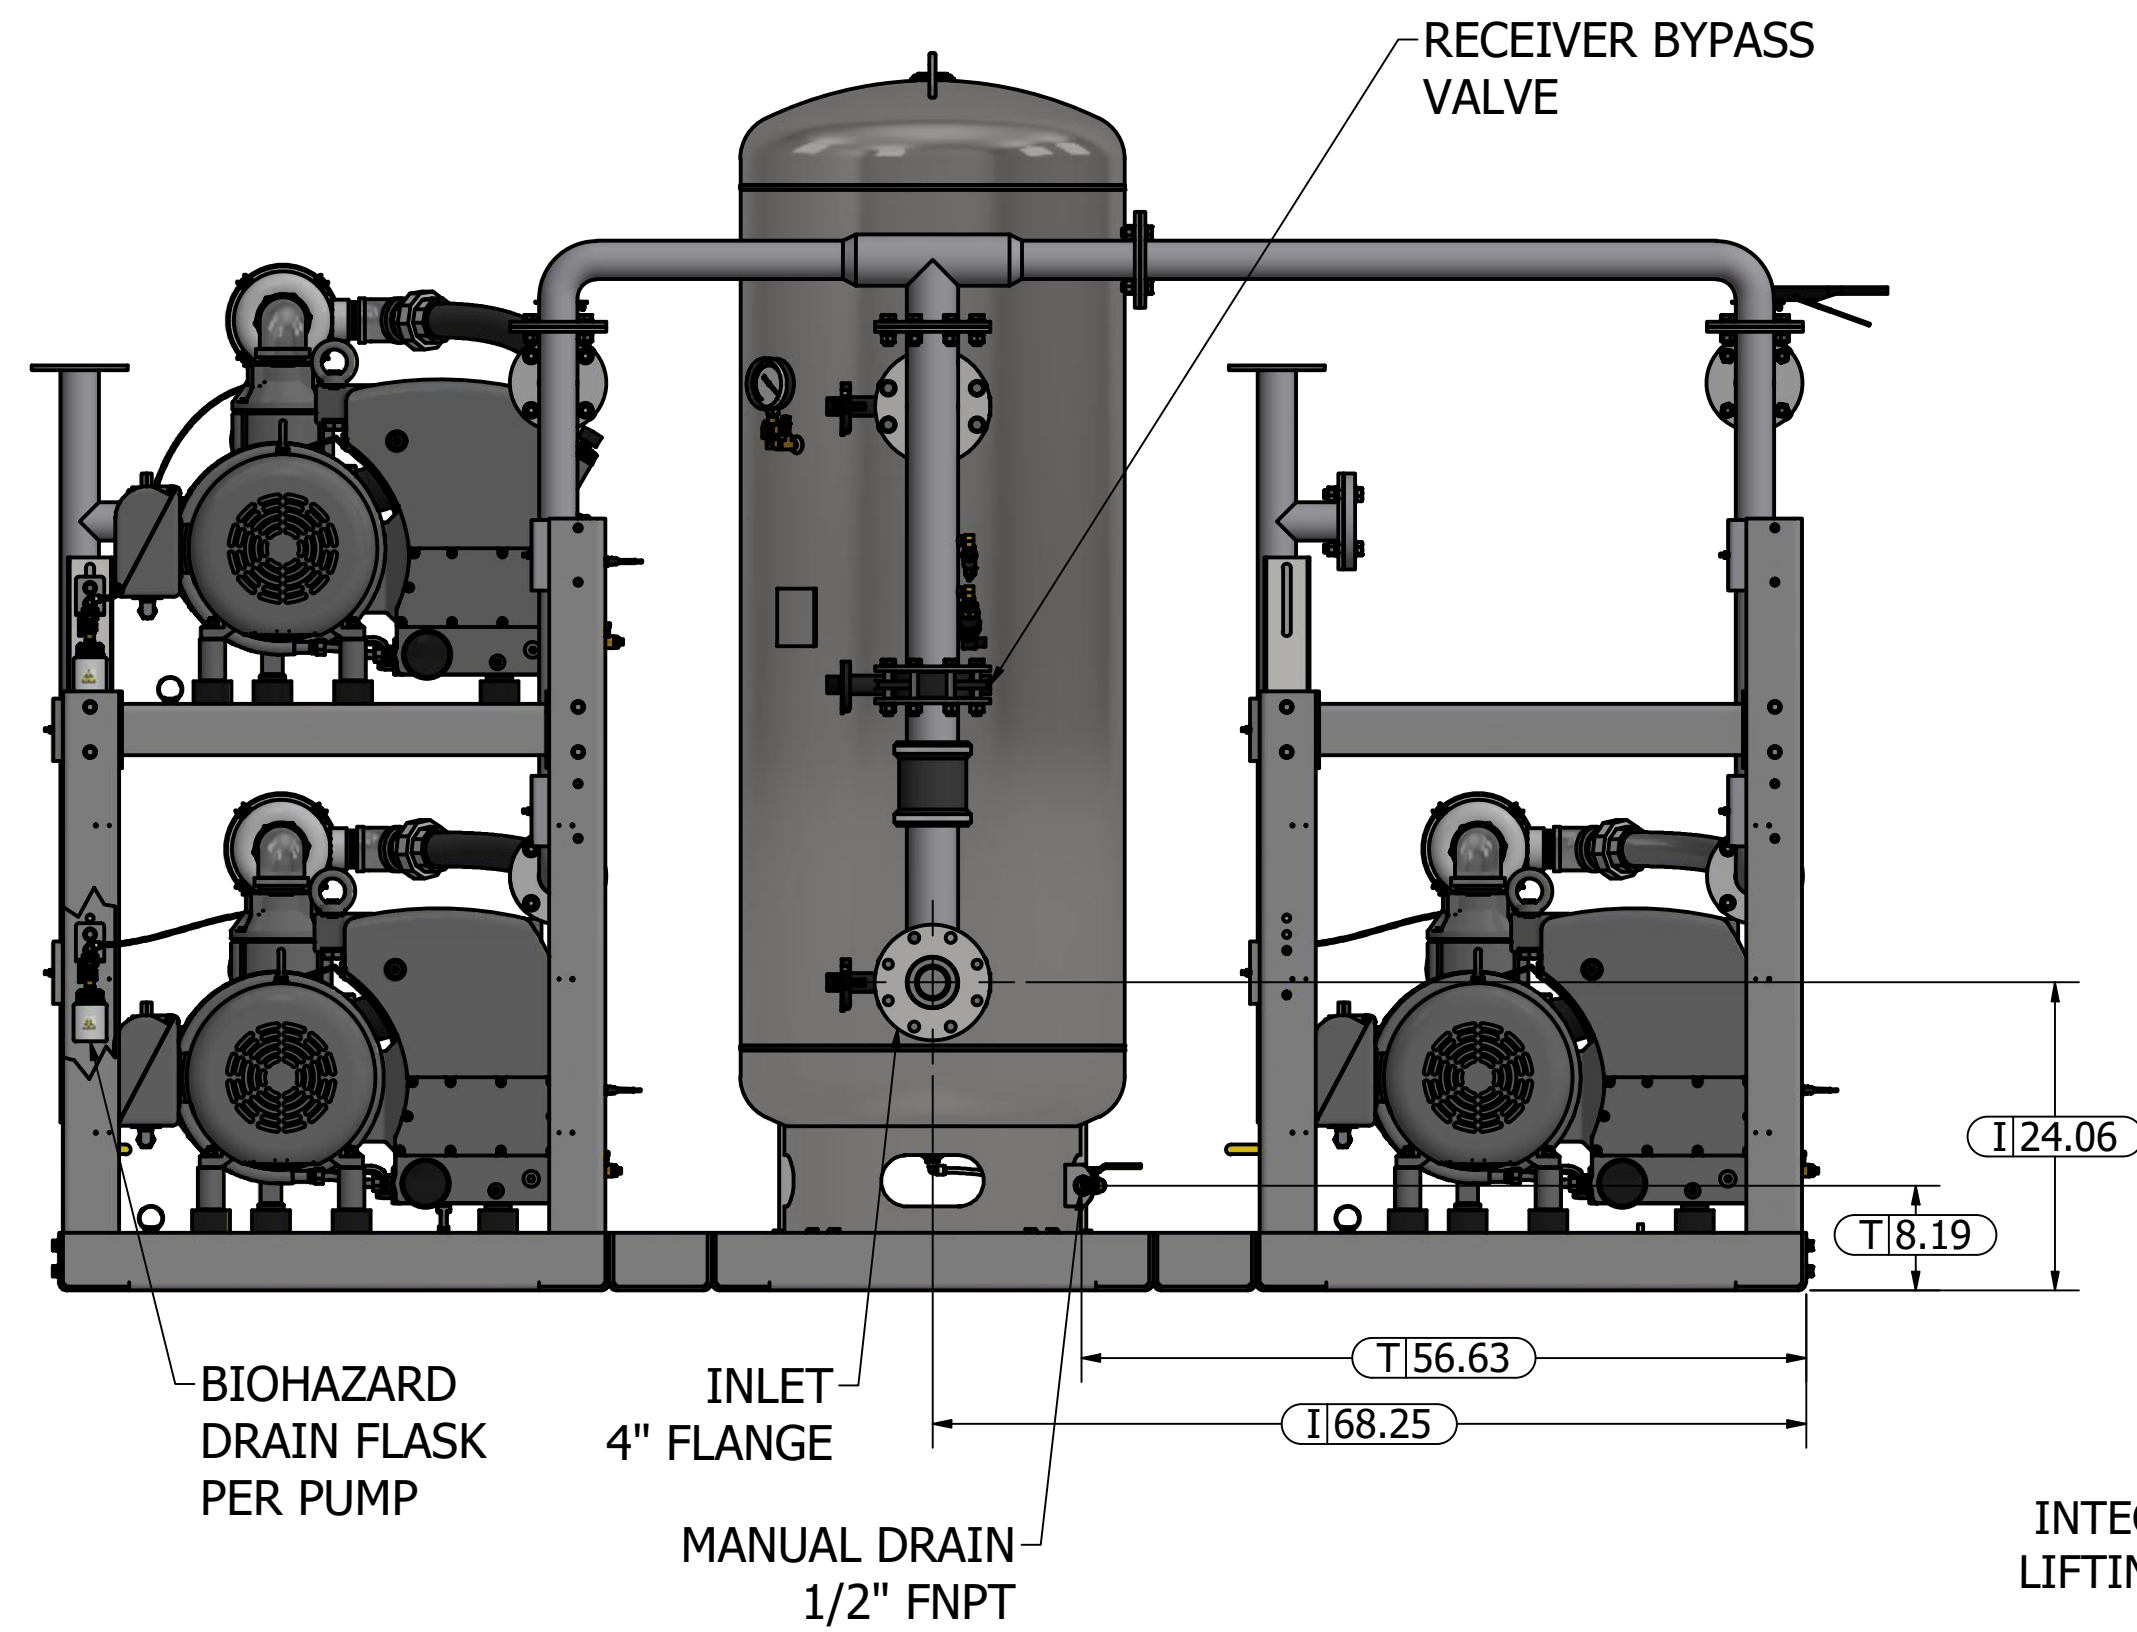

240 GALLON-
RECEIVER

INTAKE ISOLATION-
VALVE FOR FUTURE
EXPANSION PUMP



CONTROL CABINET-

HEPA INTAKE FILTER
PER PUMP

DISCHARGE
3" FLANGE
(2 PLACES)

D 72.25

MANUAL
CONDENSATE
DRAIN,TYP

Revised:	APS	Date:	3/9/2023	Drawn:	MDB	Date:	9/16/2010
 BEACON MEDICAL		This drawing and the information contained therein remain the property of BeaconMedicals and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedicals Engineering.				Scale:	
Description:		Part Number:					
GENERAL ASSEMBLY 15HP		4107 8523 00					
TX-EXP-QX LUBE VAC SPC 240G		DN:		HOP230842		Rev: 03	
RECEIVER		Sheet 1 of 1		DO NOT SCALE THIS DOCUMENT			