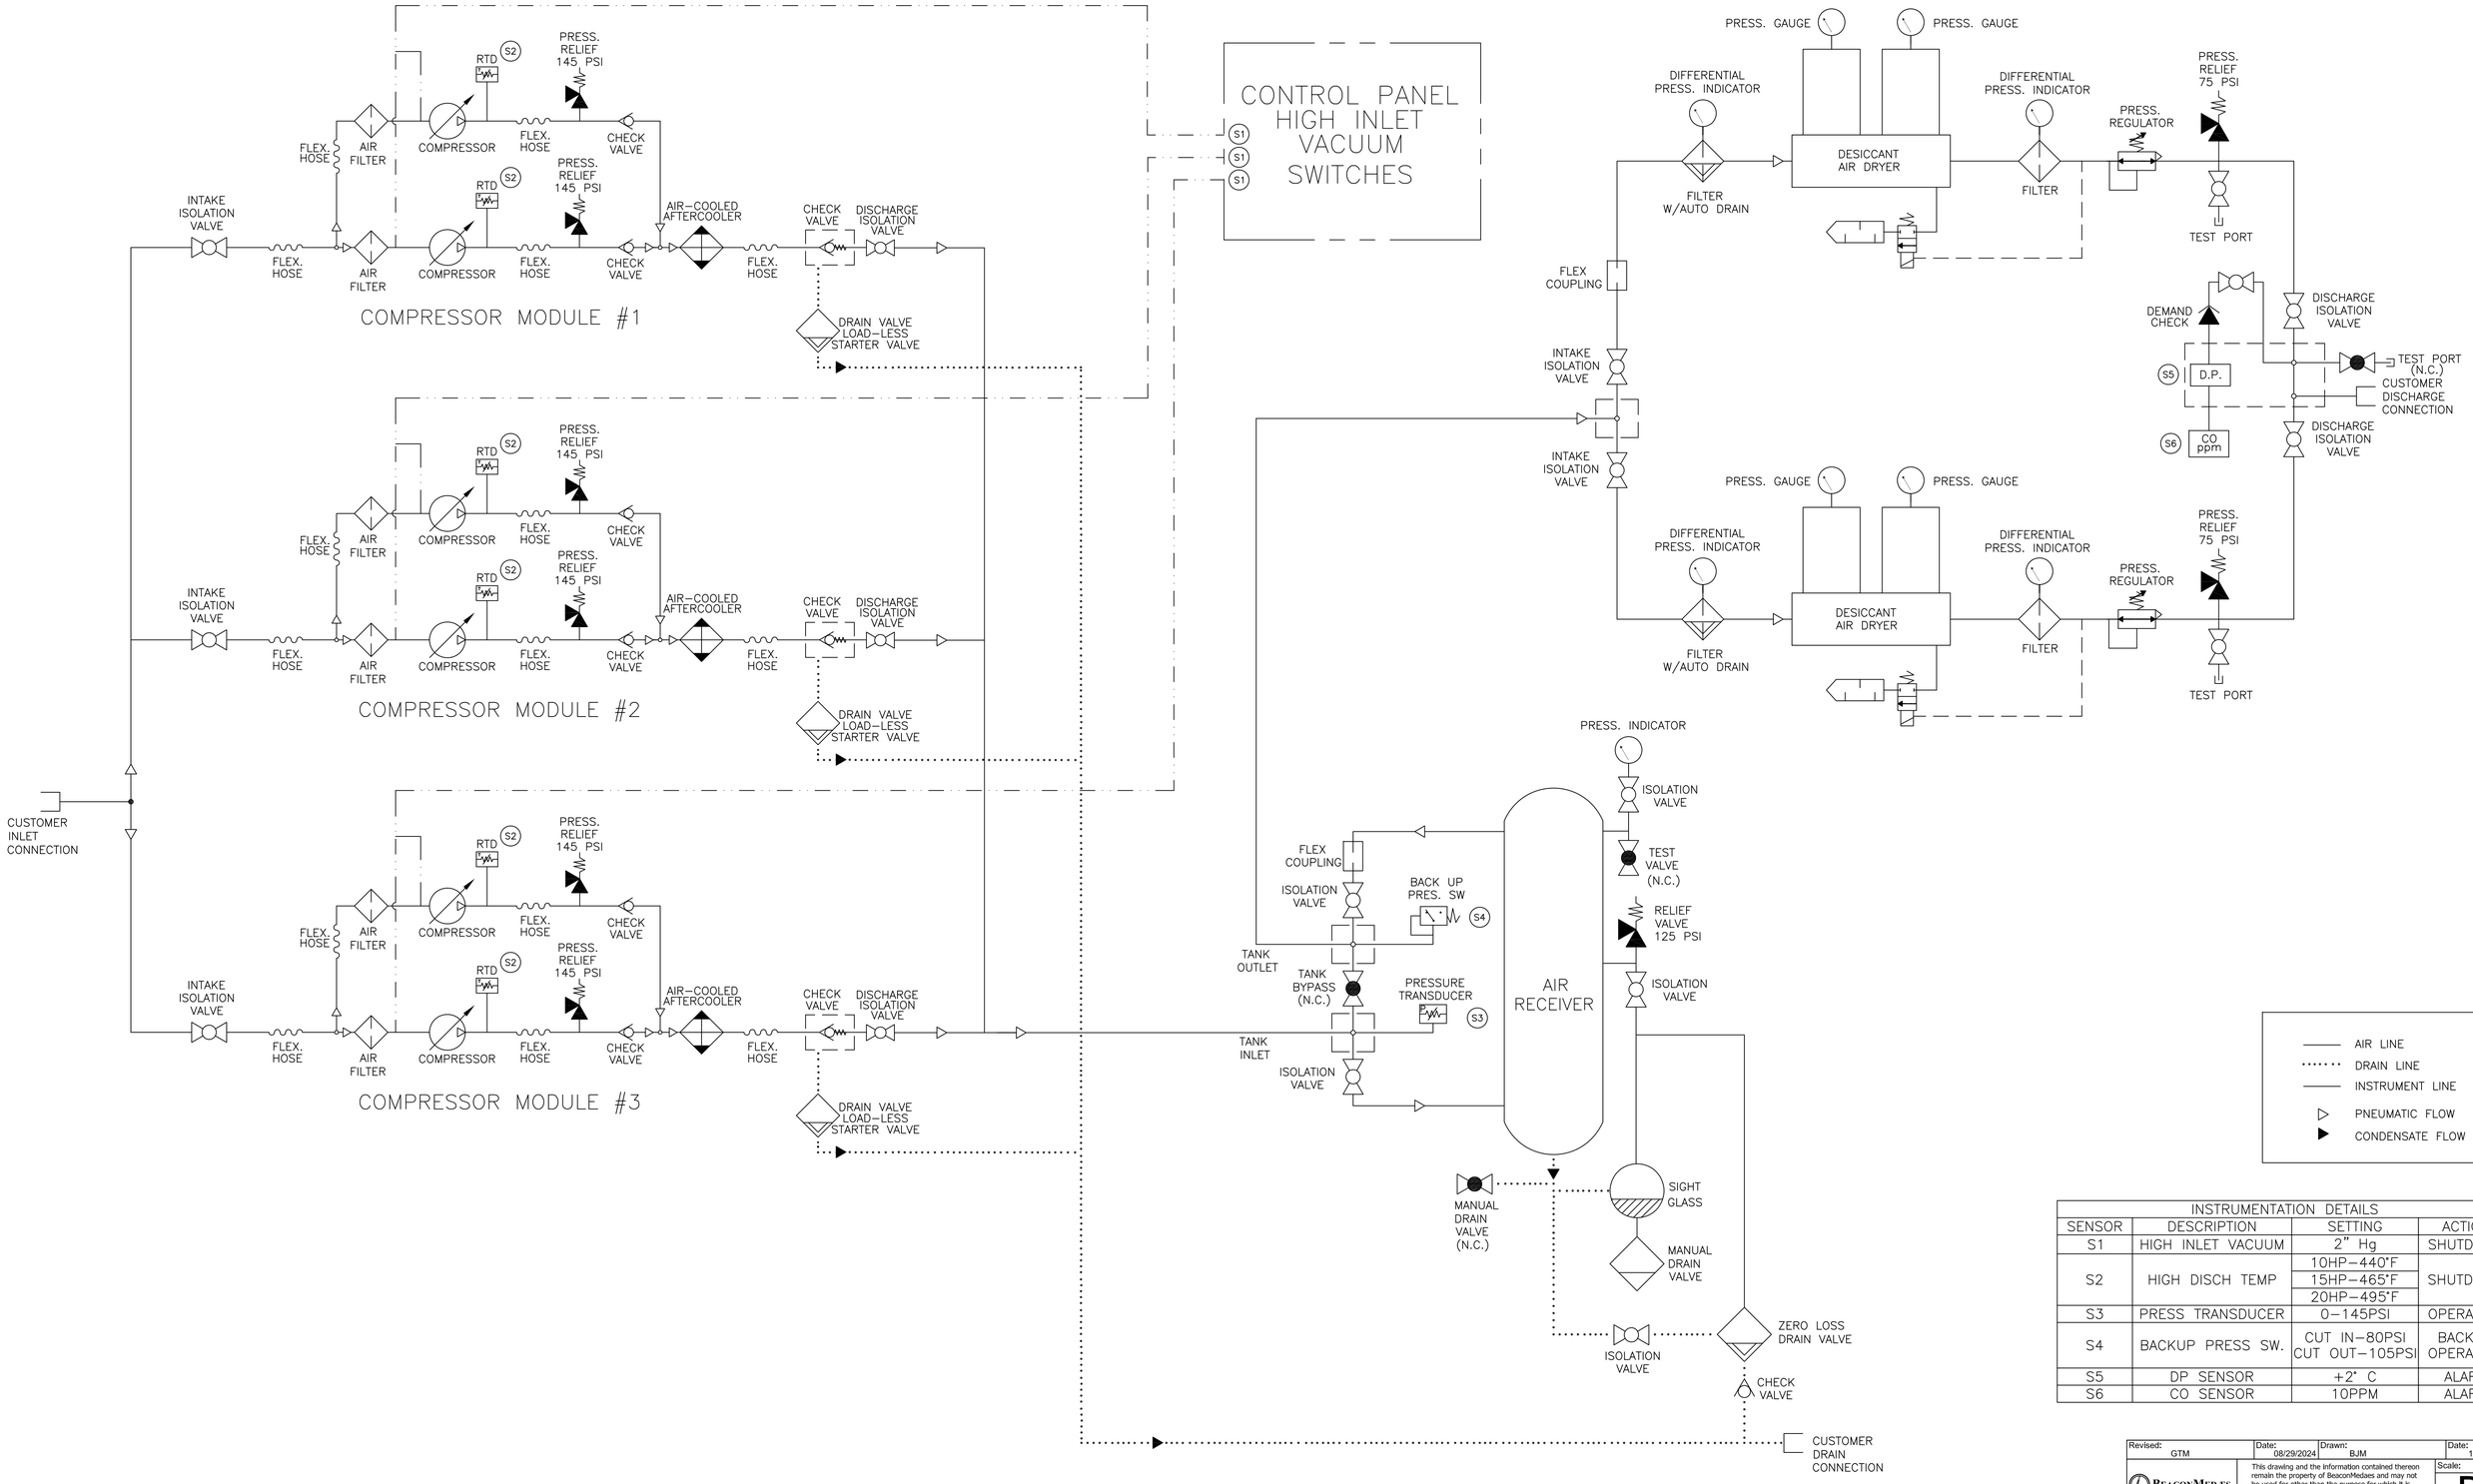

AIR LINE
DRAIN LINE
INSTRUMENT LINE
PNEUMATIC FLOW
CONDENSATE FLOW

INSTRUMENTATION DETAILS			
SENSOR	DESCRIPTION	SETTING	ACTION
S1	HIGH INLET VACUUM	2" Hg	SHUTDOWN
S2	HIGH DISCH TEMP	10HP-440°F	SHUTDOWN
		15HP-465°F	
		20HP-495°F	
S3	PRESS TRANSDUCER	0-145PSI	OPERATION
S4	BACKUP PRESS SW.	CUT IN-80PSI CUT OUT-105PSI	BACKUP OPERATION
S5	DP SENSOR	+2° C	ALARM
S6	CO SENSOR	10PPM	ALARM

Revised: GTM	Date: 08/29/2024	Drawn: BJM	Date: 12/16/2009
BeaconMedaes	This drawing and the information contained thereon remain the property of BeaconMedaes and may not be used for other than the purpose for which it is loaned without the expressed written permission from BeaconMedaes Engineering.		Scale: NTS
			D
Description: PNEUMATIC DIAGRAM TX SCROLL SPC W/DRYER (10-20HP)	Part Number: 4107 8512 03		
	DN: HOP240470		Rev: 03
	Sheet 1 of 1		DO NOT SCALE THIS DOCUMENT